




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
 Data File : VV028522.D
 Acq On : 11 Oct 2022 15:05
 Operator : SY/MD
 Sample : N5024-06ME
 Misc : 5.04g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BF6ME

Manual IntegrationsAPPROVED

Quant Time: Oct 12 00:30:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 12 00:26:27 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/12/2022
 Supervised By :Mahesh Dadoda 10/12/2022

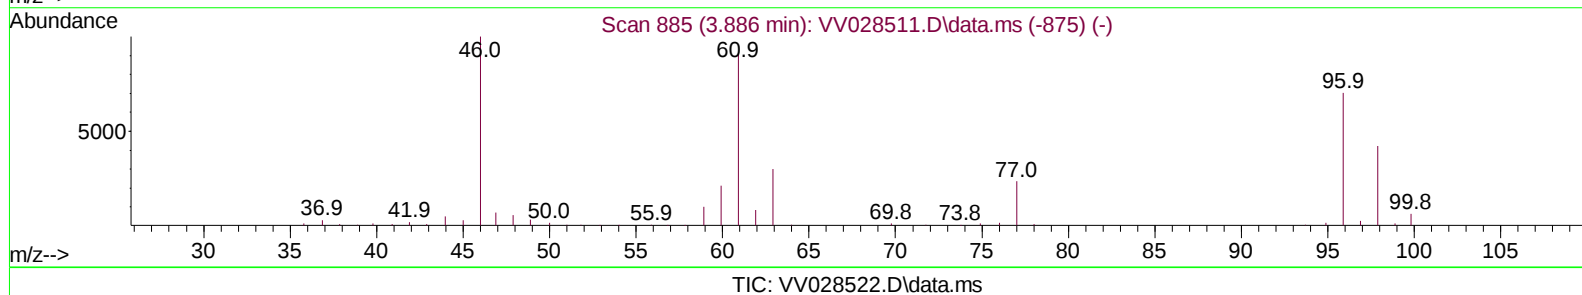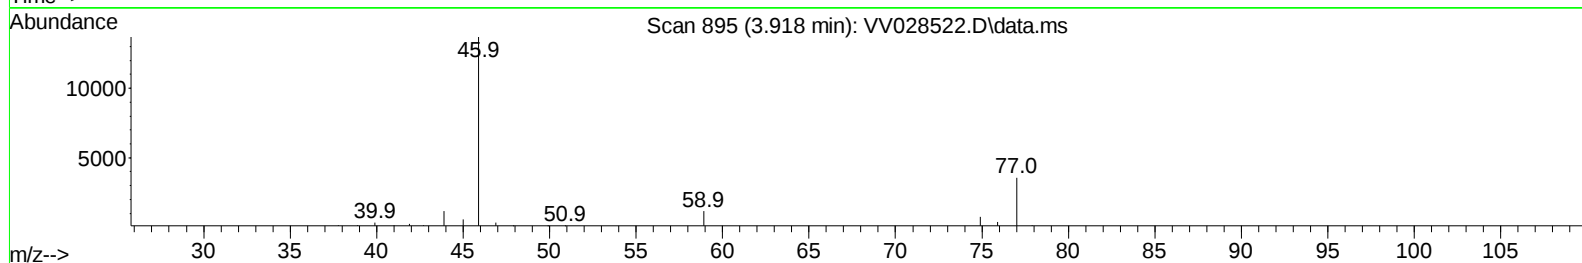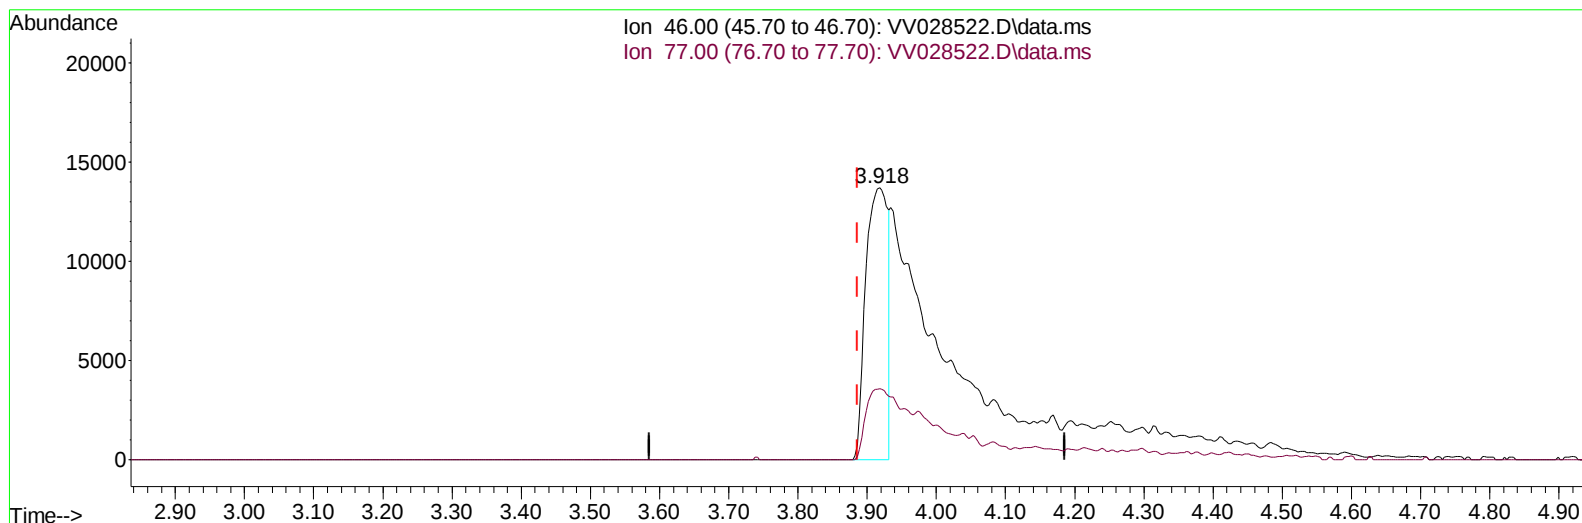

(21) 2-Butanone-d5 (S)

3.918min (+ 0.032) 17.54 ug/L

response 29853

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	22.10	27.78
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
 Data File : VV028522.D
 Acq On : 11 Oct 2022 15:05
 Operator : SY/MD
 Sample : N5024-06ME
 Misc : 5.04g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BF6ME

Manual IntegrationsAPPROVED

Quant Time: Oct 12 00:30:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 12 00:26:27 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/12/2022
 Supervised By :Mahesh Dadoda 10/12/2022

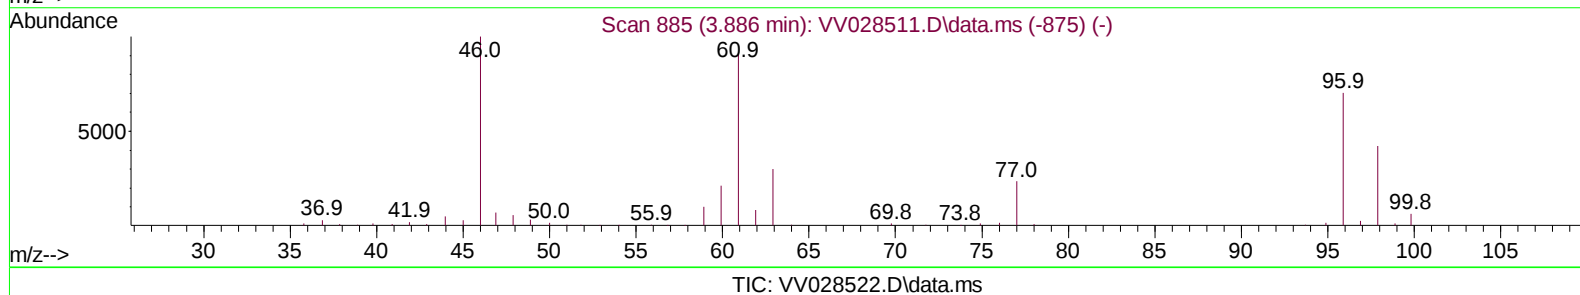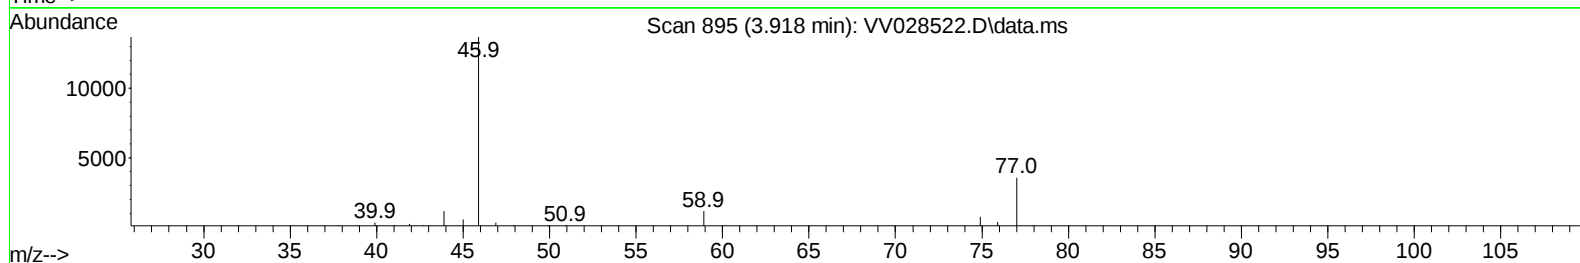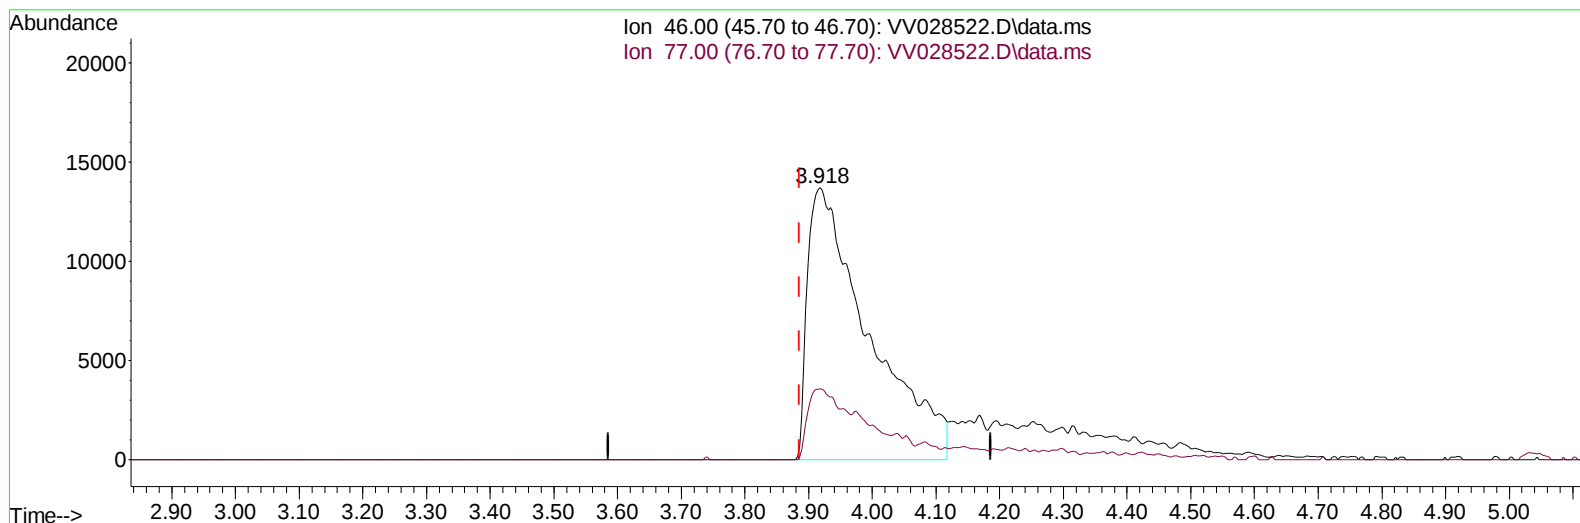

(21) 2-Butanone-d5 (S)

3.918min (+ 0.032) 53.58 ug/L m

response 91185

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	22.10	9.10#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
 Data File : VV028522.D
 Acq On : 11 Oct 2022 15:05
 Operator : SY/MD
 Sample : N5024-06ME
 Misc : 5.04g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BF6ME

Manual IntegrationsAPPROVED

Quant Time: Oct 12 00:30:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 12 00:26:27 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/12/2022
 Supervised By :Mahesh Dadoda 10/12/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	251947	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	248836	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	130301	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	57053	29.348	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	58.700%#	
7) Chloroethane-d5	1.568	69	47689	30.937	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	61.880%#	
11) 1,1-Dichloroethene-d2	2.088	63	106985	32.335	ug/L	-0.01
Spiked Amount 50.000	Range 60	- 125	Recovery	=	64.680%	
21) 2-Butanone-d5	3.918	46	91185m	53.581	ug/L	0.03
Spiked Amount 100.000	Range 40	- 130	Recovery	=	53.580%	
24) Chloroform-d	4.339	84	148061	41.527	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	83.060%	
26) 1,2-Dichloroethane-d4	5.024	65	104843	45.595	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	91.200%	
32) Benzene-d6	5.040	84	295171	37.019	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	74.040%	
36) 1,2-Dichloropropane-d6	6.066	67	88634	34.094	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	68.180%#	
41) Toluene-d8	7.310	98	284752	39.888	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	79.780%#	
43) trans-1,3-Dichloroprop...	7.619	79	52403	39.547	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	79.100%	
47) 2-Hexanone-d5	8.114	63	90625	64.082	ug/L	0.03
Spiked Amount 100.000	Range 45	- 130	Recovery	=	64.080%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	123924	34.835	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	69.660%	
66) 1,2-Dichlorobenzene-d4	11.619	152	115425	42.751	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	85.500%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
Data File : VV028522.D
Acq On : 11 Oct 2022 15:05
Operator : SY/MD
Sample : N5024-06ME
Misc : 5.04g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BF6ME

Manual IntegrationsAPPROVED

Quant Time: Oct 12 00:30:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 12 00:26:27 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/12/2022
Supervised By :Mahesh Dadoda 10/12/2022

