

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
 Data File : VV028512.D
 Acq On : 11 Oct 2022 10:41
 Operator : SY/MD
 Sample : VV1011MBL01
 Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK277

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rBV	162930	164845	13.17%	1.748%
2	1.565	157	163	177	rVB	121942	139868	11.17%	1.483%
3	2.101	322	330	348	rVB	258885	377781	30.17%	4.005%
4	2.500	447	454	456	rBV5	3142	3465	0.28%	0.037%
5	2.590	478	482	485	rVB	563	443	0.04%	0.005%
6	2.761	527	535	538	rBV4	970	1152	0.09%	0.012%
7	2.918	582	584	587	rBV3	362	237	0.02%	0.003%
8	2.950	590	594	598	rBV3	525	384	0.03%	0.004%
9	3.047	621	624	626	rBV2	435	284	0.02%	0.003%
10	3.089	635	637	642	rBV2	371	356	0.03%	0.004%
11	3.163	657	660	663	rBV3	368	264	0.02%	0.003%
12	3.262	684	691	694	rBV4	477	573	0.05%	0.006%
13	3.420	737	740	746	rVB3	487	400	0.03%	0.004%
14	3.635	805	807	812	rVB3	367	240	0.02%	0.003%
15	3.699	824	827	833	rVB3	570	376	0.03%	0.004%
16	3.748	838	842	845	rBV	433	343	0.03%	0.004%
17	3.899	878	889	930	rBV2	50972	238328	19.03%	2.527%
18	4.339	1011	1026	1056	rVB	191830	481763	38.48%	5.107%
19	4.603	1105	1108	1114	rVB4	447	315	0.03%	0.003%
20	4.654	1121	1124	1126	rBV3	666	498	0.04%	0.005%
21	4.761	1154	1157	1159	rBV	430	339	0.03%	0.004%
22	5.037	1226	1243	1273	rBV2	482931	1252140	100.00%	13.274%
23	5.384	1349	1351	1353	rBV3	589	345	0.03%	0.004%
24	5.481	1376	1381	1382	rBV3	436	340	0.03%	0.004%
25	5.523	1391	1394	1398	rBV	298	265	0.02%	0.003%
26	5.551	1399	1403	1405	rBV2	419	248	0.02%	0.003%
27	5.609	1409	1421	1458	rBV	361565	736861	58.85%	7.812%
28	5.963	1528	1531	1536	rBV4	482	450	0.04%	0.005%
29	6.063	1549	1562	1589	rBV	269042	561671	44.86%	5.954%
30	6.204	1603	1606	1609	rBV2	700	483	0.04%	0.005%
31	6.269	1623	1626	1627	rBV3	553	374	0.03%	0.004%
32	6.297	1632	1635	1637	rBV3	486	240	0.02%	0.003%
33	6.375	1655	1659	1664	rVB2	850	699	0.06%	0.007%
34	6.433	1672	1677	1682	rVB3	398	293	0.02%	0.003%
35	6.664	1747	1749	1753	rVB3	568	330	0.03%	0.003%
36	6.709	1761	1763	1768	rVB4	358	253	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
 Data File : VV028512.D
 Acq On : 11 Oct 2022 10:41
 Operator : SY/MD
 Sample : VV1011MBL01
 Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK277

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.760	1775	1779	1782	rBV	341	227	0.02%	0.002%
38	6.979	1836	1847	1874	rBV	167960	315701	25.21%	3.347%
39	7.217	1918	1921	1923	rBV3	554	392	0.03%	0.004%
40	7.307	1938	1949	1974	rBV	580136	1023030	81.70%	10.845%
41	7.561	2026	2028	2032	rVB2	430	242	0.02%	0.003%
42	7.616	2034	2045	2067	rBV2	117403	210099	16.78%	2.227%
43	7.760	2088	2090	2094	rBV2	546	309	0.02%	0.003%
44	7.924	2138	2141	2144	rBV2	475	378	0.03%	0.004%
45	7.973	2154	2156	2157	rBV	575	261	0.02%	0.003%
46	8.085	2181	2191	2233	rBV	303226	617252	49.30%	6.544%
47	8.510	2320	2323	2327	rVB2	651	456	0.04%	0.005%
48	8.622	2356	2358	2362	rVB2	700	416	0.03%	0.004%
49	8.670	2370	2373	2377	rVV3	304	245	0.02%	0.003%
50	8.780	2402	2407	2408	rBV	336	250	0.02%	0.003%
51	8.844	2415	2427	2451	rBV	527670	873590	69.77%	9.261%
52	9.092	2497	2504	2508	rVV3	535	440	0.04%	0.005%
53	9.114	2508	2511	2513	rBV3	519	258	0.02%	0.003%
54	9.146	2519	2521	2523	rBV2	633	295	0.02%	0.003%
55	9.178	2529	2531	2533	rVB2	596	245	0.02%	0.003%
56	9.198	2533	2537	2540	rVB3	377	292	0.02%	0.003%
57	9.461	2616	2619	2623	rVV3	403	317	0.03%	0.003%
58	9.484	2623	2626	2631	rVV3	428	362	0.03%	0.004%
59	9.551	2637	2647	2648	rBV4	681	936	0.07%	0.010%
60	9.992	2781	2784	2787	rBV2	362	231	0.02%	0.002%
61	10.082	2808	2812	2815	rBV	390	318	0.03%	0.003%
62	10.127	2820	2826	2830	rBV3	639	604	0.05%	0.006%
63	10.207	2839	2851	2870	rBV	343376	554748	44.30%	5.881%
64	10.371	2898	2902	2905	rBV3	340	280	0.02%	0.003%
65	10.461	2927	2930	2933	rBV2	394	250	0.02%	0.003%
66	10.532	2943	2952	2960	rBV6	1443	2466	0.20%	0.026%
67	10.612	2975	2977	2981	rVB2	552	283	0.02%	0.003%
68	10.654	2985	2990	2994	rBV3	383	384	0.03%	0.004%
69	10.731	3010	3014	3016	rBV2	544	296	0.02%	0.003%
70	10.908	3061	3069	3073	rBV5	1343	1699	0.14%	0.018%
71	10.963	3082	3086	3090	rBV2	382	318	0.03%	0.003%
72	11.056	3113	3115	3119	rVB3	519	276	0.02%	0.003%
73	11.079	3119	3122	3128	rBV3	372	355	0.03%	0.004%
74	11.182	3147	3154	3161	rBV6	2468	3297	0.26%	0.035%
75	11.239	3161	3172	3191	rBV	567673	892178	71.25%	9.458%
76	11.400	3220	3222	3224	rBV2	578	222	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
 Data File : VV028512.D
 Acq On : 11 Oct 2022 10:41
 Operator : SY/MD
 Sample : VV1011MBL01
 Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK277

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.468	3240	3243	3247	rBV2	518	462	0.04%	0.005%
78	11.506	3252	3255	3258	rBV	340	236	0.02%	0.003%
79	11.616	3276	3289	3313	rBV	570663	903855	72.18%	9.582%
80	11.831	3353	3356	3358	rBV3	374	291	0.02%	0.003%
81	11.899	3374	3377	3380	rVB2	326	251	0.02%	0.003%
82	11.985	3401	3404	3408	rBV2	363	287	0.02%	0.003%
83	12.053	3421	3425	3428	rBV2	336	283	0.02%	0.003%
84	12.101	3438	3440	3446	rBV3	354	250	0.02%	0.003%
85	12.403	3531	3534	3536	rVB3	601	259	0.02%	0.003%
86	12.423	3536	3540	3541	rBV2	674	536	0.04%	0.006%
87	12.535	3573	3575	3581	rVB2	402	293	0.02%	0.003%
88	12.577	3586	3588	3591	rBV	354	227	0.02%	0.002%
89	12.641	3600	3608	3615	rBV7	3253	4692	0.37%	0.050%
90	12.754	3638	3643	3644	rBV2	337	289	0.02%	0.003%
91	13.034	3726	3730	3732	rVV	519	349	0.03%	0.004%
92	13.050	3732	3735	3738	rVB4	386	289	0.02%	0.003%
93	13.259	3791	3800	3811	rVV5	5178	8344	0.67%	0.088%
94	13.355	3826	3830	3832	rBV2	397	321	0.03%	0.003%
95	13.497	3864	3874	3890	rBV2	15357	27503	2.20%	0.292%
96	13.648	3916	3921	3925	rBV3	509	540	0.04%	0.006%
97	13.738	3940	3949	3959	rVB4	7432	10884	0.87%	0.115%
98	13.821	3973	3975	3978	rBV	439	221	0.02%	0.002%
99	14.014	4032	4035	4036	rBV	570	346	0.03%	0.004%
100	14.304	4123	4125	4127	rBV2	730	405	0.03%	0.004%


Sum of corrected areas: 9432857

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
Data File : VV028512.D
Acq On : 11 Oct 2022 10:41
Operator : SY/MD
Sample : VV1011MBL01
Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

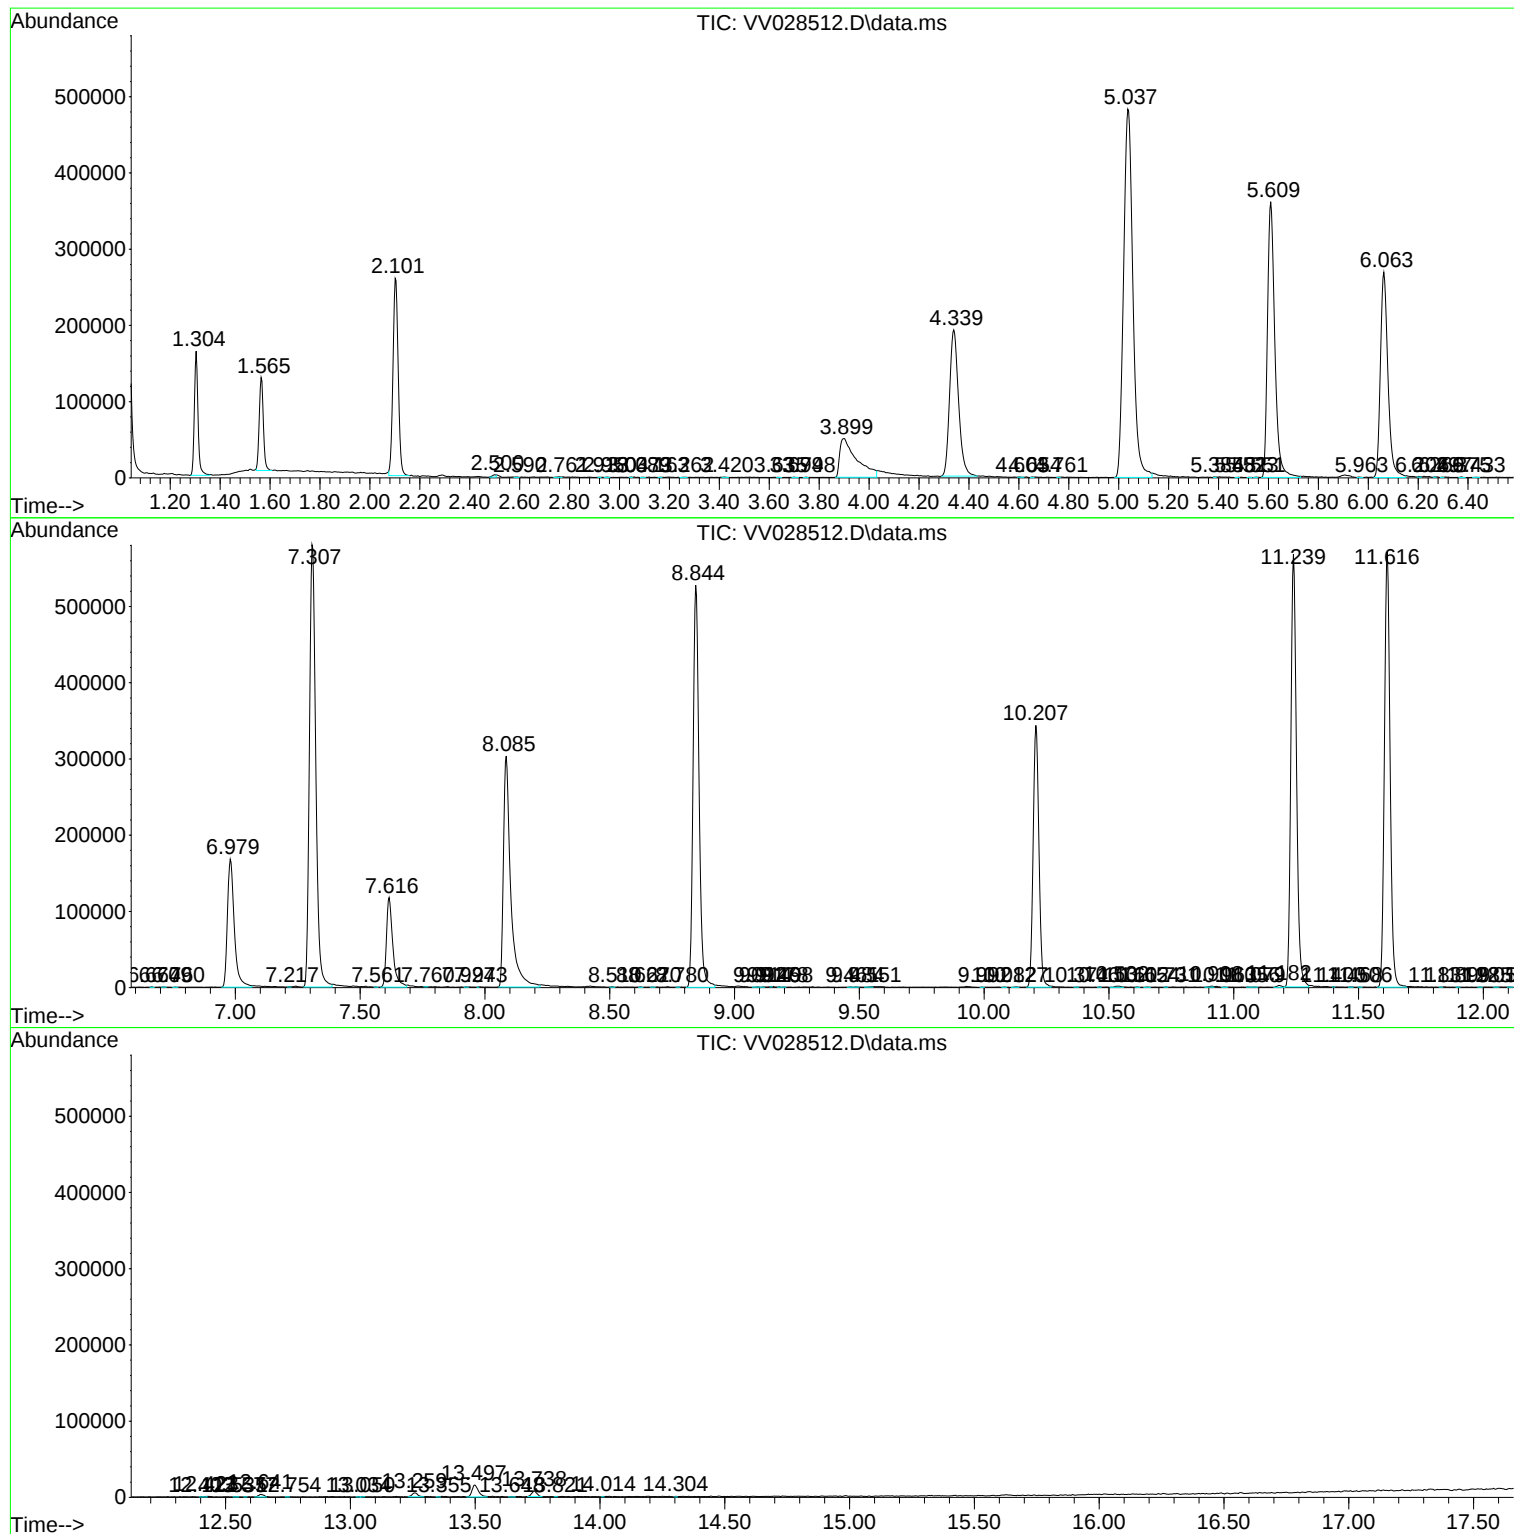

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
Data File : VV028512.D
Acq On : 11 Oct 2022 10:41
Operator : SY/MD
Sample : VV1011MBL01
Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
Data File : VV028512.D
Acq On : 11 Oct 2022 10:41
Operator : SY/MD
Sample : VV1011MBL01
Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc