

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
 Data File : VV028519.D
 Acq On : 11 Oct 2022 13:43
 Operator : SY/MD
 Sample : N5079-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	104	rBV	170232	175760	12.49%	1.743%
2	1.564	157	163	175	rVB	134090	151434	10.76%	1.502%
3	2.101	321	330	347	rVB	273429	397725	28.26%	3.945%
4	2.580	475	479	482	rBV2	278	266	0.02%	0.003%
5	2.629	492	494	499	rBV2	319	218	0.02%	0.002%
6	2.908	578	581	583	rBV2	470	220	0.02%	0.002%
7	2.979	601	603	609	rVB2	334	229	0.02%	0.002%
8	3.034	618	620	624	rVB2	598	279	0.02%	0.003%
9	3.124	645	648	650	rBV2	604	292	0.02%	0.003%
10	3.294	696	701	704	rBV3	446	357	0.03%	0.004%
11	3.375	723	726	728	rVB3	348	216	0.02%	0.002%
12	3.400	731	734	736	rBV	336	240	0.02%	0.002%
13	3.455	748	751	754	rBV	298	240	0.02%	0.002%
14	3.526	768	773	776	rBV2	348	328	0.02%	0.003%
15	3.638	806	808	812	rVV2	411	316	0.02%	0.003%
16	3.815	860	863	867	rVB2	597	491	0.03%	0.005%
17	3.899	877	889	925	rBV2	59105	267247	18.99%	2.651%
18	4.336	1010	1025	1054	rBV	212791	535893	38.07%	5.316%
19	4.802	1168	1170	1176	rVB4	611	401	0.03%	0.004%
20	4.863	1186	1189	1191	rBV3	515	381	0.03%	0.004%
21	4.905	1200	1202	1205	rBV3	420	279	0.02%	0.003%
22	4.960	1217	1219	1222	rVB3	517	211	0.01%	0.002%
23	5.037	1226	1243	1280	rBV2	544460	1407536	100.00%	13.962%
24	5.455	1368	1373	1375	rBV3	641	421	0.03%	0.004%
25	5.484	1380	1382	1385	rVB3	504	221	0.02%	0.002%
26	5.503	1385	1388	1391	rBV	438	289	0.02%	0.003%
27	5.539	1397	1399	1403	rVB2	508	307	0.02%	0.003%
28	5.564	1403	1407	1409	rBV2	606	394	0.03%	0.004%
29	5.606	1409	1420	1451	rBV	356194	737850	52.42%	7.319%
30	5.886	1504	1507	1508	rBV	1290	596	0.04%	0.006%
31	5.905	1508	1513	1515	rBV4	2564	2660	0.19%	0.026%
32	5.995	1538	1541	1543	rBV2	306	238	0.02%	0.002%
33	6.059	1548	1561	1584	rBV	299209	622651	44.24%	6.177%
34	6.294	1632	1634	1637	rBV3	311	184	0.01%	0.002%
35	6.320	1641	1642	1645	rVB	571	241	0.02%	0.002%
36	6.455	1680	1684	1686	rBV2	488	369	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
 Data File : VV028519.D
 Acq On : 11 Oct 2022 13:43
 Operator : SY/MD
 Sample : N5079-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.519	1700	1704	1706	rVB2	534	387	0.03%	0.004%
38	6.696	1754	1759	1761	rBV2	668	555	0.04%	0.006%
39	6.757	1776	1778	1782	rVB2	770	507	0.04%	0.005%
40	6.786	1785	1787	1791	rBV2	462	333	0.02%	0.003%
41	6.847	1804	1806	1808	rBV	303	210	0.01%	0.002%
42	6.873	1812	1814	1820	rVB3	556	379	0.03%	0.004%
43	6.905	1820	1824	1825	rBV	394	256	0.02%	0.003%
44	6.918	1825	1828	1829	rBV2	510	270	0.02%	0.003%
45	6.979	1836	1847	1876	rBV	184427	349681	24.84%	3.469%
46	7.307	1938	1949	1976	rBV	643230	1123697	79.83%	11.147%
47	7.616	2035	2045	2069	rBV	126645	230603	16.38%	2.288%
48	7.760	2088	2090	2091	rBV	661	209	0.01%	0.002%
49	7.860	2117	2121	2129	rBV6	564	706	0.05%	0.007%
50	7.960	2148	2152	2155	rVB3	652	447	0.03%	0.004%
51	8.037	2169	2176	2181	rBV2	523	563	0.04%	0.006%
52	8.082	2181	2190	2225	rBV	331123	678930	48.24%	6.735%
53	8.320	2262	2264	2265	rVB	684	185	0.01%	0.002%
54	8.416	2292	2294	2295	rBV	506	225	0.02%	0.002%
55	8.603	2350	2352	2361	rBV4	466	483	0.03%	0.005%
56	8.699	2378	2382	2383	rBV	444	336	0.02%	0.003%
57	8.728	2387	2391	2394	rBV3	450	355	0.03%	0.004%
58	8.767	2401	2403	2407	rBV2	312	225	0.02%	0.002%
59	8.792	2407	2411	2414	rBV2	607	496	0.04%	0.005%
60	8.844	2416	2427	2458	rBV	521390	865071	61.46%	8.581%
61	9.120	2512	2513	2517	rVB2	646	313	0.02%	0.003%
62	9.149	2517	2522	2532	rBV4	653	1032	0.07%	0.010%
63	9.201	2536	2538	2543	rBV3	547	433	0.03%	0.004%
64	9.387	2593	2596	2598	rBV	368	211	0.01%	0.002%
65	9.400	2598	2600	2602	rVB2	388	189	0.01%	0.002%
66	9.461	2616	2619	2623	rVB3	404	308	0.02%	0.003%
67	9.487	2623	2627	2630	rBV	296	301	0.02%	0.003%
68	9.638	2670	2674	2675	rBV2	437	257	0.02%	0.003%
69	9.709	2694	2696	2699	rVV	310	232	0.02%	0.002%
70	9.921	2758	2762	2765	rBV3	476	323	0.02%	0.003%
71	9.956	2769	2773	2774	rBV2	360	226	0.02%	0.002%
72	10.017	2789	2792	2794	rBV2	392	233	0.02%	0.002%
73	10.207	2840	2851	2870	rBV	390979	613589	43.59%	6.087%
74	10.368	2899	2901	2906	rBV3	487	312	0.02%	0.003%
75	10.477	2927	2935	2945	rVB7	3951	7005	0.50%	0.069%
76	10.535	2951	2953	2955	rBV2	565	258	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
 Data File : VV028519.D
 Acq On : 11 Oct 2022 13:43
 Operator : SY/MD
 Sample : N5079-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	10.587	2967	2969	2971	rVB	489	184	0.01%	0.002%
78	10.635	2979	2984	2986	rBV4	423	439	0.03%	0.004%
79	10.802	3034	3036	3040	rBV2	363	258	0.02%	0.003%
80	10.969	3085	3088	3091	rBV	515	323	0.02%	0.003%
81	11.178	3149	3153	3156	rVB	398	290	0.02%	0.003%
82	11.239	3160	3172	3195	rBV	563423	890949	63.30%	8.838%
83	11.432	3230	3232	3235	rBV2	603	225	0.02%	0.002%
84	11.615	3275	3289	3307	rBV	630019	995976	70.76%	9.880%
85	11.918	3380	3383	3386	rBV2	473	340	0.02%	0.003%
86	12.004	3405	3410	3412	rBV2	508	261	0.02%	0.003%
87	12.230	3477	3480	3484	rVB2	586	392	0.03%	0.004%
88	12.255	3484	3488	3491	rBV	542	315	0.02%	0.003%
89	12.300	3499	3502	3505	rBV	764	331	0.02%	0.003%
90	12.381	3524	3527	3528	rBV2	350	214	0.02%	0.002%
91	12.564	3581	3584	3586	rBV2	441	216	0.02%	0.002%
92	12.641	3604	3608	3609	rBV	449	329	0.02%	0.003%
93	12.937	3697	3700	3702	rBV2	427	207	0.01%	0.002%
94	12.979	3711	3713	3716	rBV	485	281	0.02%	0.003%
95	13.033	3726	3730	3734	rBV2	361	378	0.03%	0.004%
96	13.149	3764	3766	3771	rBV2	368	288	0.02%	0.003%
97	13.766	3956	3958	3961	rBV3	438	325	0.02%	0.003%
98	13.834	3976	3979	3983	rBV4	692	485	0.03%	0.005%
99	13.959	4016	4018	4020	rVB2	561	221	0.02%	0.002%
100	14.326	4130	4132	4135	rBV2	617	415	0.03%	0.004%




Sum of corrected areas: 10080953

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
Data File : VV028519.D
Acq On : 11 Oct 2022 13:43
Operator : SY/MD
Sample : N5079-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

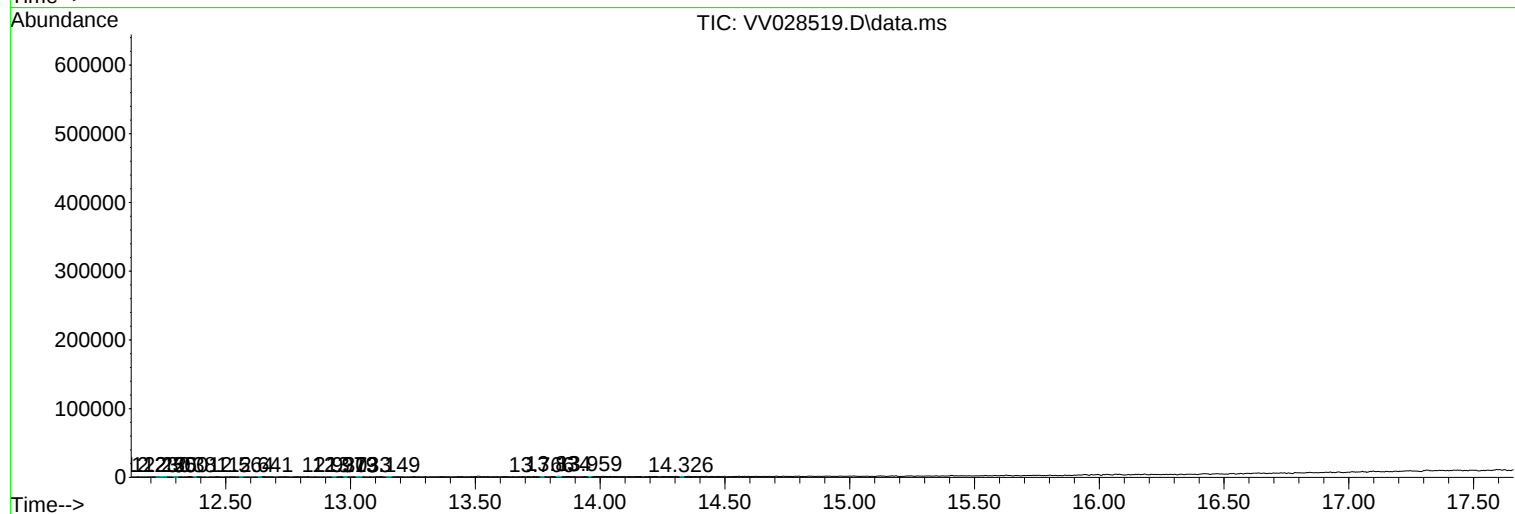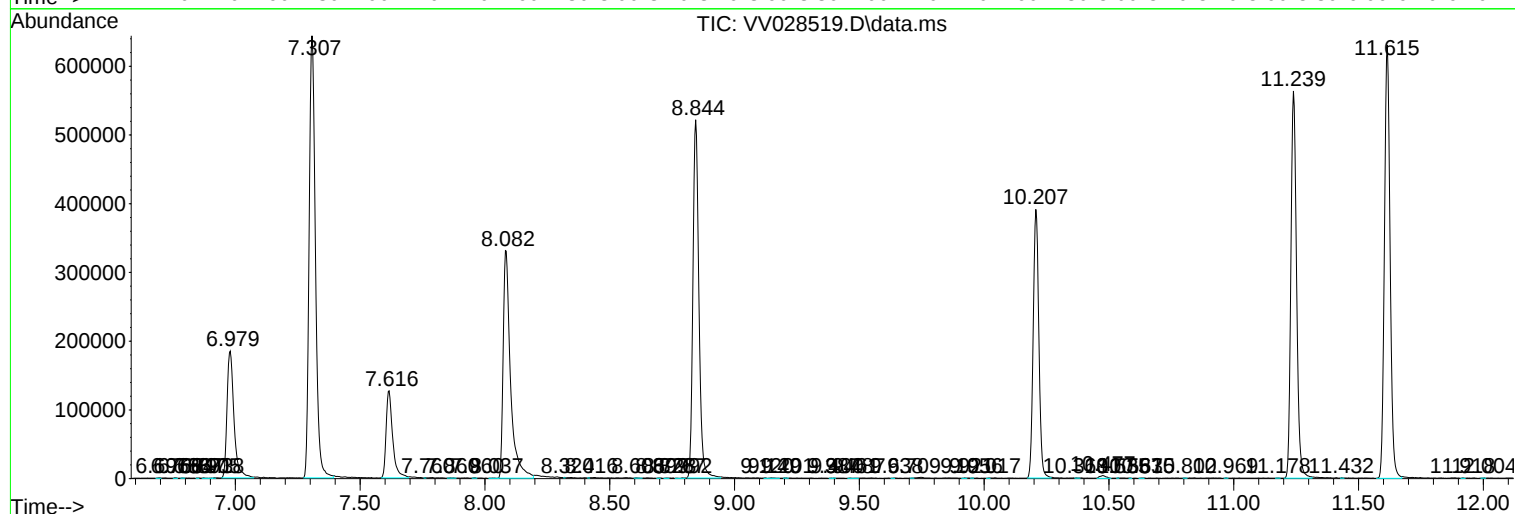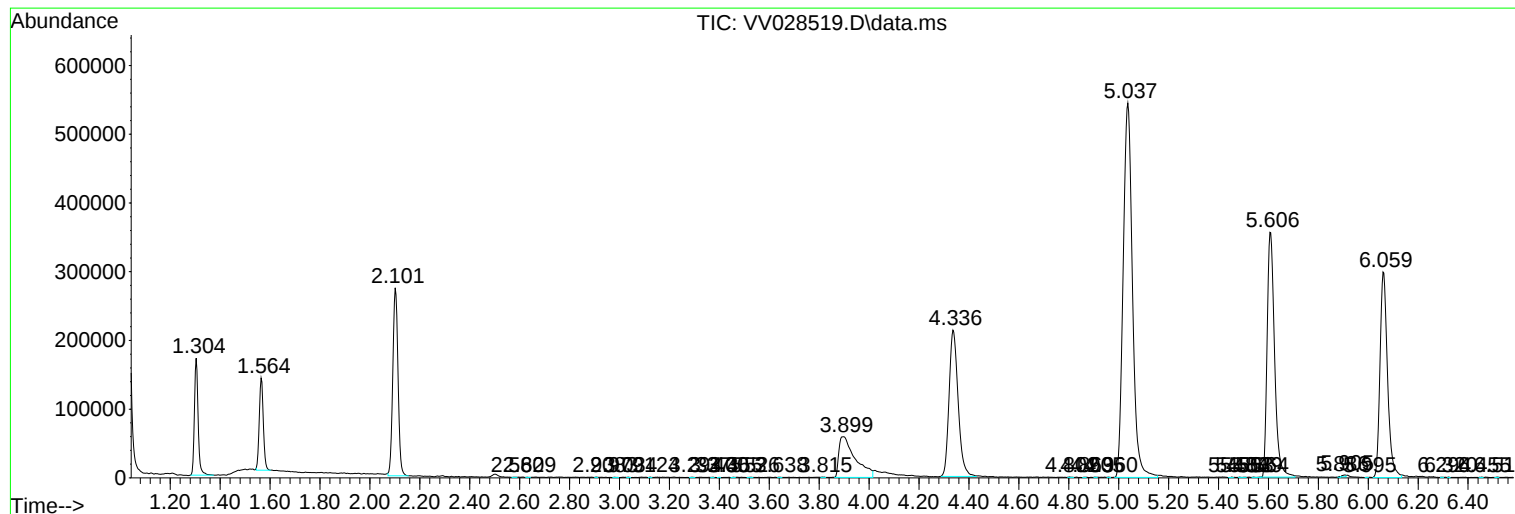

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
Data File : VV028519.D
Acq On : 11 Oct 2022 13:43
Operator : SY/MD
Sample : N5079-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
Data File : VV028519.D
Acq On : 11 Oct 2022 13:43
Operator : SY/MD
Sample : N5079-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc