

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
 Data File : VV028520.D
 Acq On : 11 Oct 2022 14:17
 Operator : SY/MD
 Sample : N5024-02ME
 Misc : 4.95g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBE8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	106	rBV	67274	98085	9.23%	1.197%
2	1.564	158	163	185	rVB	46277	74321	6.99%	0.907%
3	2.092	319	327	344	rVB	244045	347292	32.67%	4.239%
4	3.072	630	632	635	rVB2	463	220	0.02%	0.003%
5	3.127	647	649	652	rBV	345	213	0.02%	0.003%
6	3.484	758	760	764	rBV2	254	184	0.02%	0.002%
7	3.690	820	824	827	rVB	319	236	0.02%	0.003%
8	3.918	883	895	898	rBV2	27664	49517	4.66%	0.604%
9	4.333	1013	1024	1052	rVB	157587	404592	38.06%	4.938%
10	4.741	1147	1151	1156	rBV2	358	469	0.04%	0.006%
11	4.806	1169	1171	1179	rVB3	356	367	0.03%	0.004%
12	4.844	1179	1183	1186	rBV2	215	198	0.02%	0.002%
13	4.863	1187	1189	1194	rVB3	539	339	0.03%	0.004%
14	4.889	1194	1197	1199	rBV2	357	242	0.02%	0.003%
15	4.944	1210	1214	1217	rVV3	383	319	0.03%	0.004%
16	5.034	1225	1242	1280	rBV2	417684	1063119	100.00%	12.975%
17	5.278	1314	1318	1324	rBV3	685	756	0.07%	0.009%
18	5.333	1324	1335	1338	rBV6	4691	7231	0.68%	0.088%
19	5.606	1408	1420	1449	rBV	324259	675399	63.53%	8.243%
20	5.838	1488	1492	1494	rBV3	533	494	0.05%	0.006%
21	5.905	1504	1513	1522	rBV8	4198	9027	0.85%	0.110%
22	6.059	1550	1561	1589	rVB	222300	470657	44.27%	5.744%
23	6.365	1654	1656	1659	rVB2	351	187	0.02%	0.002%
24	6.400	1664	1667	1670	rBV	514	399	0.04%	0.005%
25	6.455	1681	1684	1687	rVB2	741	420	0.04%	0.005%
26	6.471	1687	1689	1694	rVB2	462	254	0.02%	0.003%
27	6.497	1694	1697	1699	rBV	373	242	0.02%	0.003%
28	6.539	1704	1710	1713	rBV2	390	395	0.04%	0.005%
29	6.641	1733	1742	1747	rBV6	2730	4839	0.46%	0.059%
30	6.838	1801	1803	1807	rBV3	515	301	0.03%	0.004%
31	6.979	1836	1847	1874	rBV	137839	279476	26.29%	3.411%
32	7.162	1901	1904	1908	rBV2	748	549	0.05%	0.007%
33	7.307	1938	1949	1976	rBV	490646	885964	83.34%	10.813%
34	7.616	2036	2045	2079	rBV	92081	191484	18.01%	2.337%
35	7.850	2116	2118	2121	rBV	502	234	0.02%	0.003%
36	7.883	2126	2128	2131	rVB3	408	204	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
 Data File : VV028520.D
 Acq On : 11 Oct 2022 14:17
 Operator : SY/MD
 Sample : N5024-02ME
 Misc : 4.95g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBE8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	7.928	2141	2142	2149	rVB3	624	610	0.06%	0.007%
38	7.963	2149	2153	2155	rVV3	555	422	0.04%	0.005%
39	7.976	2155	2157	2160	rVB3	864	448	0.04%	0.005%
40	8.117	2184	2201	2230	rBV2	133423	489804	46.07%	5.978%
41	8.651	2364	2367	2370	rBV2	645	493	0.05%	0.006%
42	8.744	2393	2396	2402	rVB3	567	482	0.05%	0.006%
43	8.773	2402	2405	2407	rBV2	371	263	0.02%	0.003%
44	8.847	2415	2428	2453	rBV	449885	843559	79.35%	10.295%
45	9.040	2486	2488	2489	rBV2	499	198	0.02%	0.002%
46	9.075	2497	2499	2500	rBV	526	252	0.02%	0.003%
47	9.111	2508	2510	2514	rBV3	445	358	0.03%	0.004%
48	9.182	2529	2532	2534	rBV3	749	382	0.04%	0.005%
49	9.198	2534	2537	2545	rVV3	1041	1333	0.13%	0.016%
50	9.272	2556	2560	2562	rBV2	524	365	0.03%	0.004%
51	9.294	2565	2567	2569	rBV3	422	201	0.02%	0.002%
52	9.603	2659	2663	2668	rVB3	367	285	0.03%	0.003%
53	9.632	2668	2672	2674	rBV2	360	251	0.02%	0.003%
54	9.764	2711	2713	2717	rVB2	651	395	0.04%	0.005%
55	9.892	2747	2753	2754	rBV	282	273	0.03%	0.003%
56	9.905	2754	2757	2761	rVV2	372	289	0.03%	0.004%
57	9.992	2781	2784	2786	rBV2	380	258	0.02%	0.003%
58	10.030	2791	2796	2798	rBV2	395	313	0.03%	0.004%
59	10.217	2840	2854	2877	rVV	278079	500171	47.05%	6.104%
60	10.339	2890	2892	2895	rBV2	524	193	0.02%	0.002%
61	10.390	2907	2908	2911	rVB3	658	259	0.02%	0.003%
62	10.416	2915	2916	2919	rBV2	358	221	0.02%	0.003%
63	10.461	2928	2930	2933	rVV2	537	255	0.02%	0.003%
64	10.481	2933	2936	2939	rVV3	697	546	0.05%	0.007%
65	10.532	2949	2952	2955	rBV2	210	198	0.02%	0.002%
66	10.574	2955	2965	2977	rBV6	4872	7771	0.73%	0.095%
67	10.693	3000	3002	3005	rVB	433	201	0.02%	0.002%
68	10.831	3042	3045	3048	rBV3	384	289	0.03%	0.004%
69	10.860	3051	3054	3063	rBV3	733	742	0.07%	0.009%
70	10.899	3063	3066	3070	rBV	244	199	0.02%	0.002%
71	11.008	3098	3100	3104	rVV2	414	258	0.02%	0.003%
72	11.108	3129	3131	3134	rBV	523	242	0.02%	0.003%
73	11.246	3163	3174	3195	rBV	561998	897635	84.43%	10.955%
74	11.419	3225	3228	3230	rBV2	413	300	0.03%	0.004%
75	11.571	3273	3275	3277	rBV	415	244	0.02%	0.003%
76	11.619	3278	3290	3316	rVV	540639	857389	80.65%	10.464%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
 Data File : VV028520.D
 Acq On : 11 Oct 2022 14:17
 Operator : SY/MD
 Sample : N5024-02ME
 Misc : 4.95g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BE8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.776	3332	3339	3340	rBV3	1212	1099	0.10%	0.013%
78	12.008	3407	3411	3417	rBV2	491	497	0.05%	0.006%
79	12.037	3417	3420	3422	rBV2	457	252	0.02%	0.003%
80	12.111	3440	3443	3446	rBV2	403	278	0.03%	0.003%
81	12.310	3502	3505	3506	rBV	423	209	0.02%	0.003%
82	12.497	3557	3563	3568	rBV5	789	866	0.08%	0.011%
83	12.596	3589	3594	3597	rVB3	441	400	0.04%	0.005%
84	12.641	3606	3608	3609	rBV	535	198	0.02%	0.002%
85	12.689	3618	3623	3628	rBV3	490	473	0.04%	0.006%
86	12.879	3674	3682	3688	rBV5	1164	1896	0.18%	0.023%
87	13.172	3771	3773	3776	rBV2	565	329	0.03%	0.004%
88	13.278	3802	3806	3808	rBV2	371	279	0.03%	0.003%
89	13.352	3826	3829	3833	rVB	430	359	0.03%	0.004%
90	13.506	3872	3877	3887	rVB5	1350	2138	0.20%	0.026%
91	13.657	3922	3924	3926	rVB	617	333	0.03%	0.004%
92	13.702	3936	3938	3942	rBV2	468	236	0.02%	0.003%
93	13.757	3953	3955	3959	rBV3	727	530	0.05%	0.006%
94	13.892	3990	3997	4004	rBV7	1699	2471	0.23%	0.030%
95	13.966	4018	4020	4024	rVB3	592	352	0.03%	0.004%
96	14.101	4060	4062	4066	rBV2	491	253	0.02%	0.003%
97	14.168	4081	4083	4084	rBV2	538	199	0.02%	0.002%
98	14.400	4148	4155	4156	rBV2	666	777	0.07%	0.009%
99	14.831	4285	4289	4298	rBV5	1607	2017	0.19%	0.025%
100	14.940	4320	4323	4326	rBV3	951	573	0.05%	0.007%




Sum of corrected areas: 8193586

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
Data File : VV028520.D
Acq On : 11 Oct 2022 14:17
Operator : SY/MD
Sample : N5024-02ME
Misc : 4.95g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

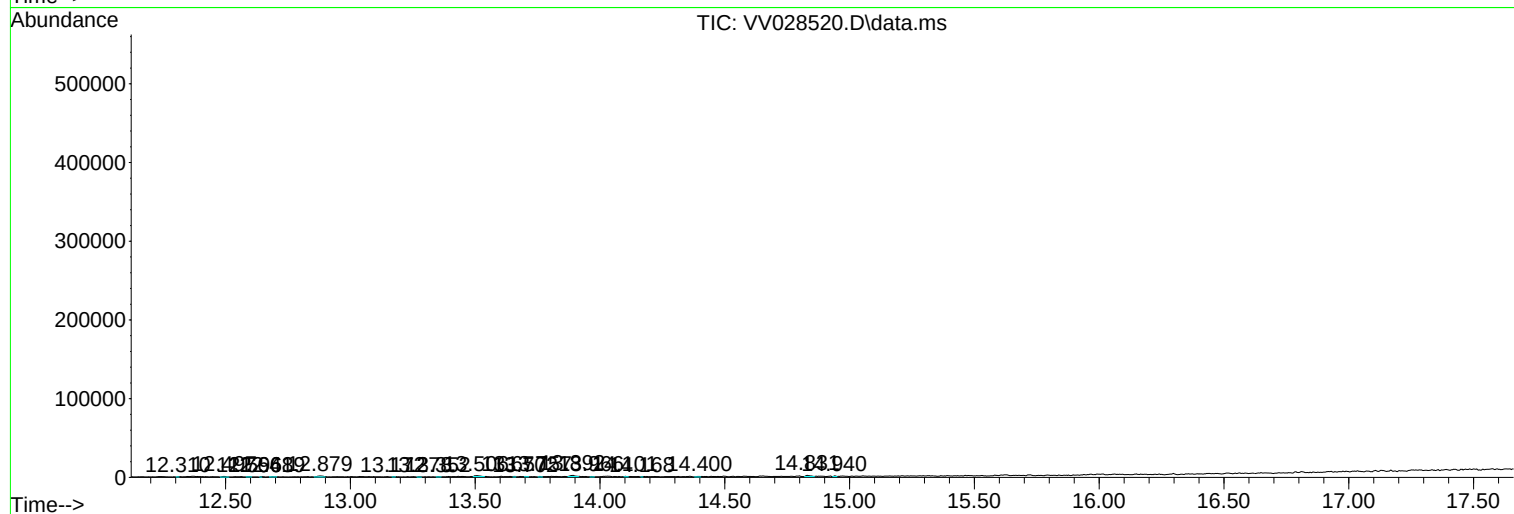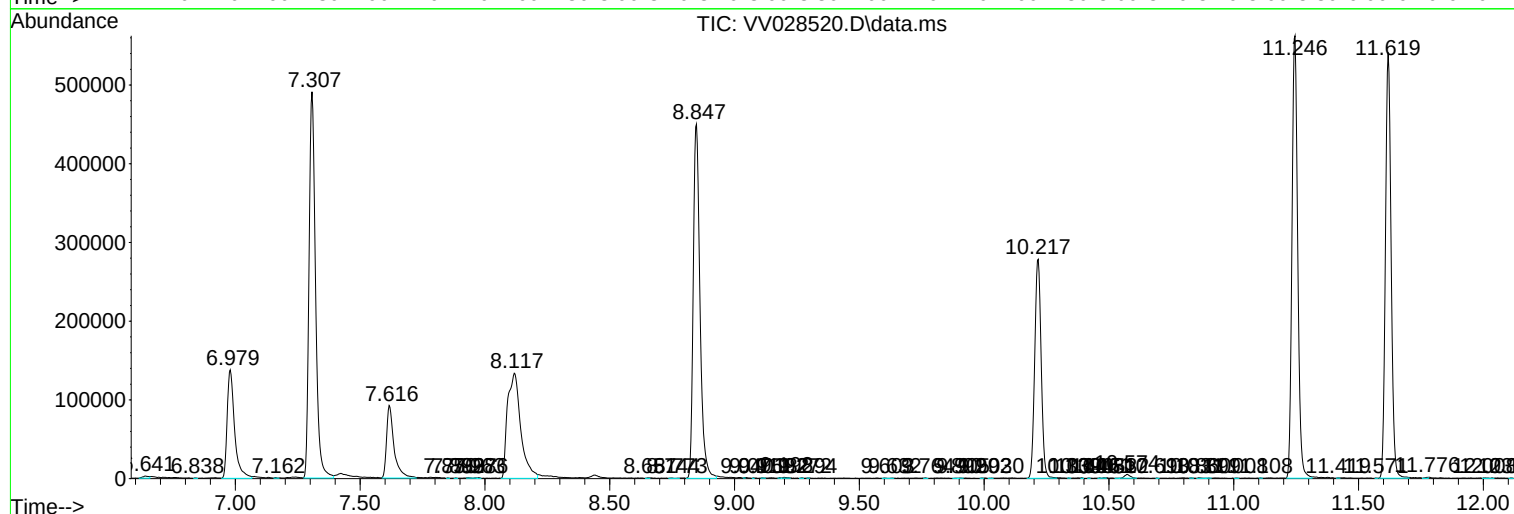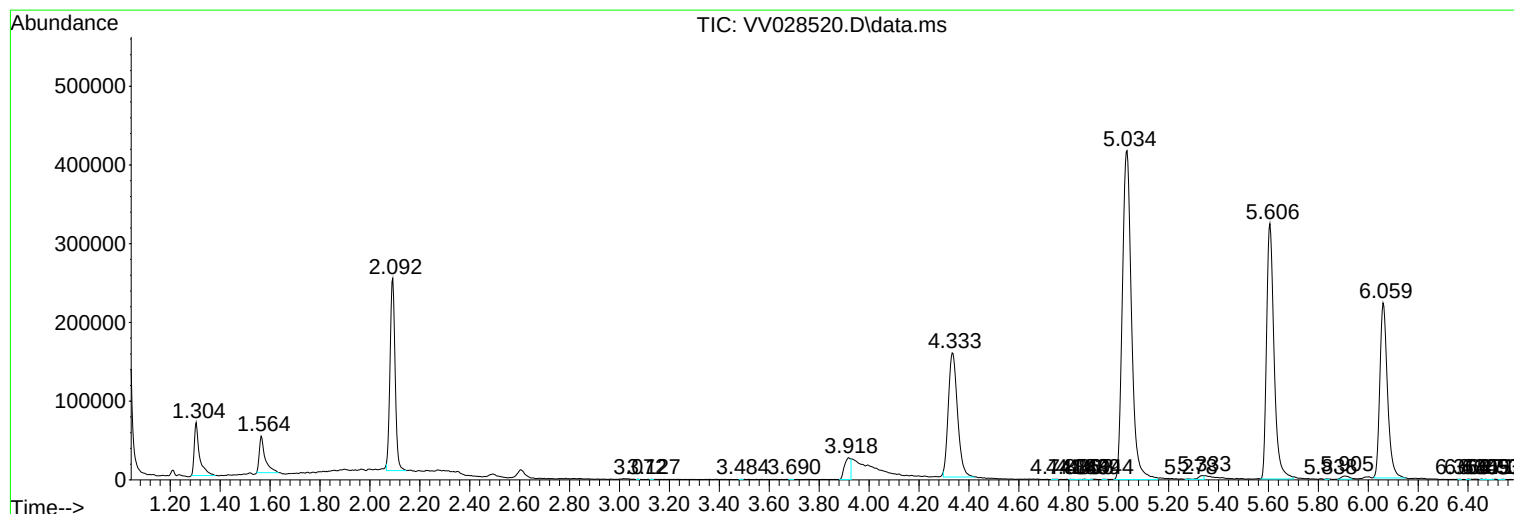

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
Data File : VV028520.D
Acq On : 11 Oct 2022 14:17
Operator : SY/MD
Sample : N5024-02ME
Misc : 4.95g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
Data File : VV028520.D
Acq On : 11 Oct 2022 14:17
Operator : SY/MD
Sample : N5024-02ME
Misc : 4.95g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc