

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
 Data File : VV028521.D
 Acq On : 11 Oct 2022 14:41
 Operator : SY/MD
 Sample : N5024-05ME
 Misc : 6.55g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BF4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	106	rBV	60174	85457	9.18%	1.222%
2	1.565	158	163	183	rBV	39101	61576	6.61%	0.881%
3	2.092	319	327	341	rVB	223931	313715	33.70%	4.486%
4	3.076	629	633	636	rBV2	229	184	0.02%	0.003%
5	3.227	677	680	682	rBV	195	132	0.01%	0.002%
6	3.269	691	693	700	rBV2	162	109	0.01%	0.002%
7	3.327	709	711	717	rVB	215	130	0.01%	0.002%
8	3.368	720	724	730	rVB3	623	716	0.08%	0.010%
9	3.400	730	734	735	rBV2	324	219	0.02%	0.003%
10	3.417	737	739	741	rVB	365	136	0.01%	0.002%
11	3.465	751	754	757	rBV2	297	212	0.02%	0.003%
12	3.536	773	776	778	rBV2	234	155	0.02%	0.002%
13	3.597	792	795	799	rBV2	194	167	0.02%	0.002%
14	3.658	812	814	821	rVB3	388	309	0.03%	0.004%
15	3.738	836	839	841	rBV	413	198	0.02%	0.003%
16	3.786	851	854	857	rBV2	210	160	0.02%	0.002%
17	3.818	862	864	867	rBV	207	131	0.01%	0.002%
18	3.921	885	896	900	rBV2	23601	46281	4.97%	0.662%
19	4.757	1154	1156	1158	rBV	175	115	0.01%	0.002%
20	4.802	1168	1170	1172	rVB	336	139	0.01%	0.002%
21	4.818	1172	1175	1177	rBV2	376	296	0.03%	0.004%
22	4.915	1203	1205	1206	rBV	246	119	0.01%	0.002%
23	4.953	1215	1217	1220	rVB3	396	160	0.02%	0.002%
24	5.037	1226	1243	1276	rBV3	367454	931019	100.00%	13.313%
25	5.609	1410	1421	1456	rBV	296939	621628	66.77%	8.889%
26	5.908	1507	1514	1515	rBV5	2969	3312	0.36%	0.047%
27	5.995	1536	1541	1542	rBV5	1908	1817	0.20%	0.026%
28	6.063	1551	1562	1584	rVB	192992	405527	43.56%	5.799%
29	6.285	1626	1631	1635	rVB4	505	493	0.05%	0.007%
30	6.416	1670	1672	1675	rBV2	340	206	0.02%	0.003%
31	6.436	1675	1678	1682	rBV3	386	274	0.03%	0.004%
32	6.455	1682	1684	1685	rBV2	336	146	0.02%	0.002%
33	6.503	1695	1699	1701	rVB	315	200	0.02%	0.003%
34	6.580	1721	1723	1726	rBV3	235	141	0.02%	0.002%
35	6.648	1732	1744	1750	rBV8	2163	4773	0.51%	0.068%
36	6.770	1781	1782	1786	rBV4	526	263	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101122\
 Data File : VW028521.D
 Acq On : 11 Oct 2022 14:41
 Operator : SY/MD
 Sample : N5024-05ME
 Misc : 6.55g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BF4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.799	1790	1791	1796	rVB4	421	207	0.02%	0.003%
38	6.860	1808	1810	1814	rBV	353	212	0.02%	0.003%
39	6.905	1821	1824	1827	rVB	311	210	0.02%	0.003%
40	6.937	1831	1834	1836	rBV	370	171	0.02%	0.002%
41	6.982	1837	1848	1879	rBV	123236	248906	26.73%	3.559%
42	7.195	1911	1914	1915	rBV2	296	156	0.02%	0.002%
43	7.233	1922	1926	1929	rBV3	692	536	0.06%	0.008%
44	7.310	1938	1950	1976	rBV	434591	784590	84.27%	11.219%
45	7.619	2035	2046	2067	rBV	81243	167992	18.04%	2.402%
46	7.876	2123	2126	2128	rBV3	190	138	0.01%	0.002%
47	7.895	2130	2132	2135	rBV	341	217	0.02%	0.003%
48	7.976	2155	2157	2158	rBV	293	117	0.01%	0.002%
49	8.037	2171	2176	2178	rVB3	272	231	0.02%	0.003%
50	8.114	2184	2200	2233	rBV3	140984	473715	50.88%	6.774%
51	8.542	2330	2333	2335	rBV2	486	307	0.03%	0.004%
52	8.629	2358	2360	2362	rBV2	308	125	0.01%	0.002%
53	8.683	2371	2377	2382	rVB3	289	456	0.05%	0.007%
54	8.709	2382	2385	2388	rBV	238	172	0.02%	0.002%
55	8.847	2416	2428	2462	rBV	422292	786905	84.52%	11.252%
56	9.236	2546	2549	2553	rBV2	198	161	0.02%	0.002%
57	9.259	2553	2556	2559	rBV	261	146	0.02%	0.002%
58	9.297	2566	2568	2571	rBV2	217	117	0.01%	0.002%
59	9.420	2604	2606	2611	rVB3	187	121	0.01%	0.002%
60	9.731	2701	2703	2706	rBV2	191	127	0.01%	0.002%
61	9.767	2711	2714	2717	rBV2	370	241	0.03%	0.003%
62	9.802	2723	2725	2728	rVB	280	126	0.01%	0.002%
63	10.053	2800	2803	2805	rBV	213	109	0.01%	0.002%
64	10.111	2819	2821	2829	rVB2	318	312	0.03%	0.004%
65	10.149	2829	2833	2834	rBV2	266	151	0.02%	0.002%
66	10.169	2838	2839	2841	rBV2	291	146	0.02%	0.002%
67	10.217	2841	2854	2874	rBV	264623	459633	49.37%	6.573%
68	10.516	2944	2947	2953	rBV2	501	436	0.05%	0.006%
69	10.577	2958	2966	2975	rVV3	3896	5396	0.58%	0.077%
70	10.664	2991	2993	2995	rBV	312	111	0.01%	0.002%
71	10.837	3043	3047	3049	rVB3	535	292	0.03%	0.004%
72	10.876	3056	3059	3062	rVB2	535	328	0.04%	0.005%
73	10.924	3071	3074	3077	rBV2	406	355	0.04%	0.005%
74	10.989	3092	3094	3097	rBV	424	193	0.02%	0.003%
75	11.098	3125	3128	3132	rBV	293	233	0.03%	0.003%
76	11.117	3132	3134	3137	rBV2	296	147	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
 Data File : VV028521.D
 Acq On : 11 Oct 2022 14:41
 Operator : SY/MD
 Sample : N5024-05ME
 Misc : 6.55g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BF4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M

Title : VOC Analysis

77	11.246	3162	3174	3192	rBV	520217	816852	87.74%	11.681%
78	11.529	3258	3262	3265	rBV2	397	328	0.04%	0.005%
79	11.619	3278	3290	3318	rBV	469702	756837	81.29%	10.822%
80	11.799	3344	3346	3349	rVB3	494	272	0.03%	0.004%
81	11.828	3352	3355	3356	rVV2	355	191	0.02%	0.003%
82	11.895	3373	3376	3377	rBV2	188	113	0.01%	0.002%
83	12.130	3446	3449	3451	rBV	303	194	0.02%	0.003%
84	12.233	3478	3481	3482	rBV	434	238	0.03%	0.003%
85	12.333	3510	3512	3515	rVB3	366	157	0.02%	0.002%
86	12.387	3527	3529	3533	rBV3	351	223	0.02%	0.003%
87	12.448	3546	3548	3553	rBV2	218	187	0.02%	0.003%
88	12.670	3614	3617	3619	rBV	240	128	0.01%	0.002%
89	12.751	3640	3642	3646	rVB3	401	213	0.02%	0.003%
90	12.889	3682	3685	3686	rBV	324	143	0.02%	0.002%
91	12.992	3715	3717	3720	rVB2	327	131	0.01%	0.002%
92	13.075	3740	3743	3745	rBV2	313	238	0.03%	0.003%
93	13.249	3795	3797	3800	rBV2	302	222	0.02%	0.003%
94	13.400	3841	3844	3846	rBV	367	171	0.02%	0.002%
95	13.596	3904	3905	3908	rVB	419	160	0.02%	0.002%
96	13.615	3908	3911	3913	rVB2	296	141	0.02%	0.002%
97	13.953	4013	4016	4019	rBV2	544	416	0.04%	0.006%
98	14.011	4032	4034	4035	rBV2	626	251	0.03%	0.004%
99	14.140	4072	4074	4076	rBV2	481	294	0.03%	0.004%
100	14.178	4084	4086	4089	rBV	509	264	0.03%	0.004%




Sum of corrected areas: 6993223

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
Data File : VV028521.D
Acq On : 11 Oct 2022 14:41
Operator : SY/MD
Sample : N5024-05ME
Misc : 6.55g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BF4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

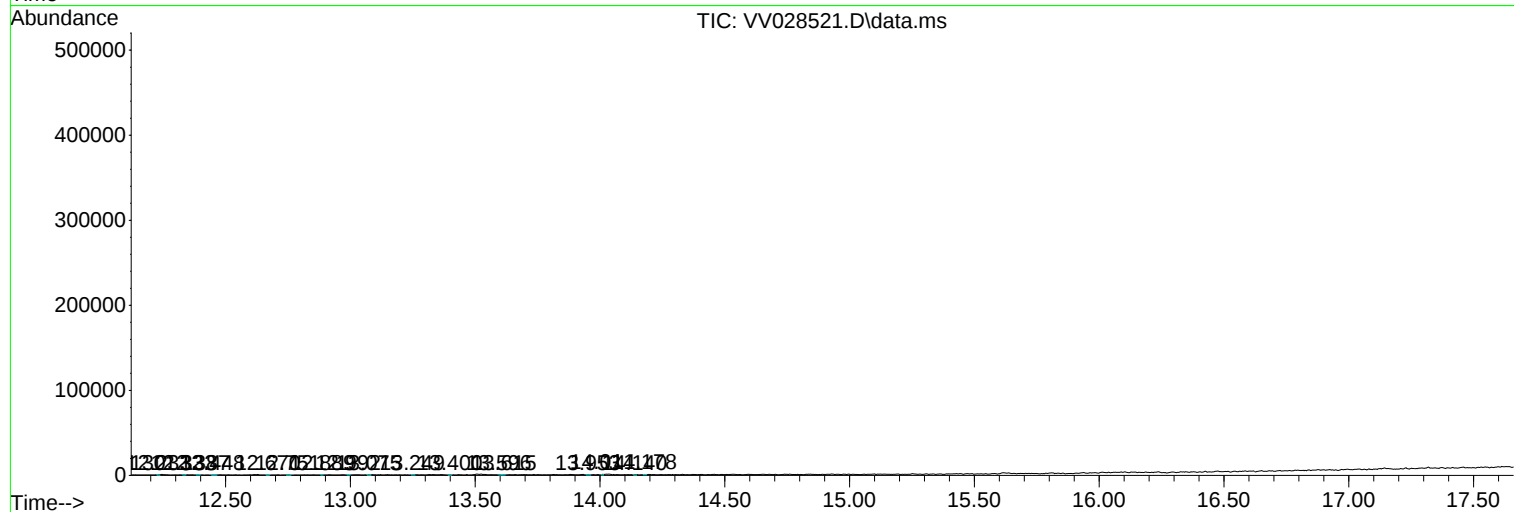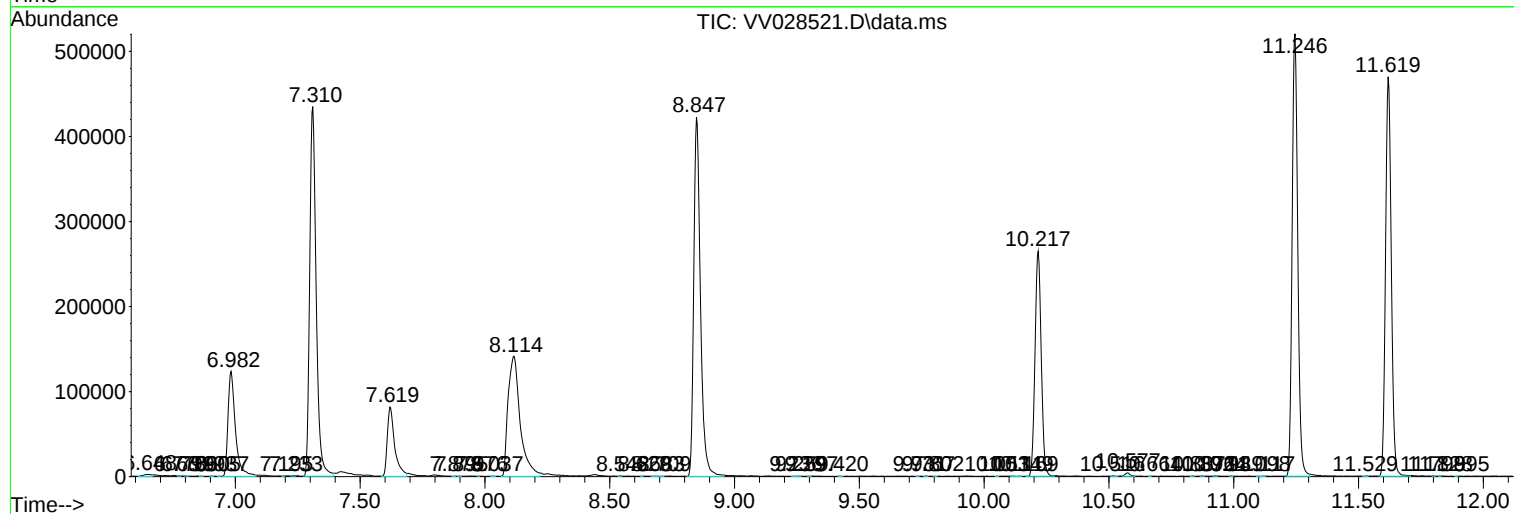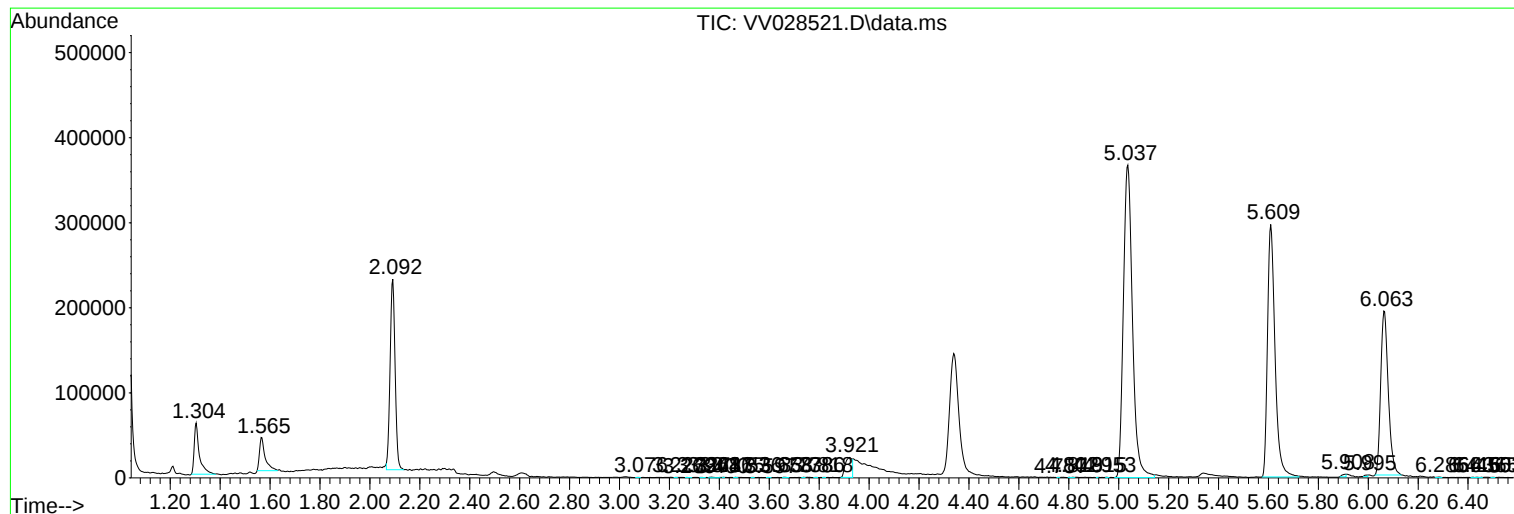

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
Data File : VV028521.D
Acq On : 11 Oct 2022 14:41
Operator : SY/MD
Sample : N5024-05ME
Misc : 6.55g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BF4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
Data File : VV028521.D
Acq On : 11 Oct 2022 14:41
Operator : SY/MD
Sample : N5024-05ME
Misc : 6.55g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BF4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc