
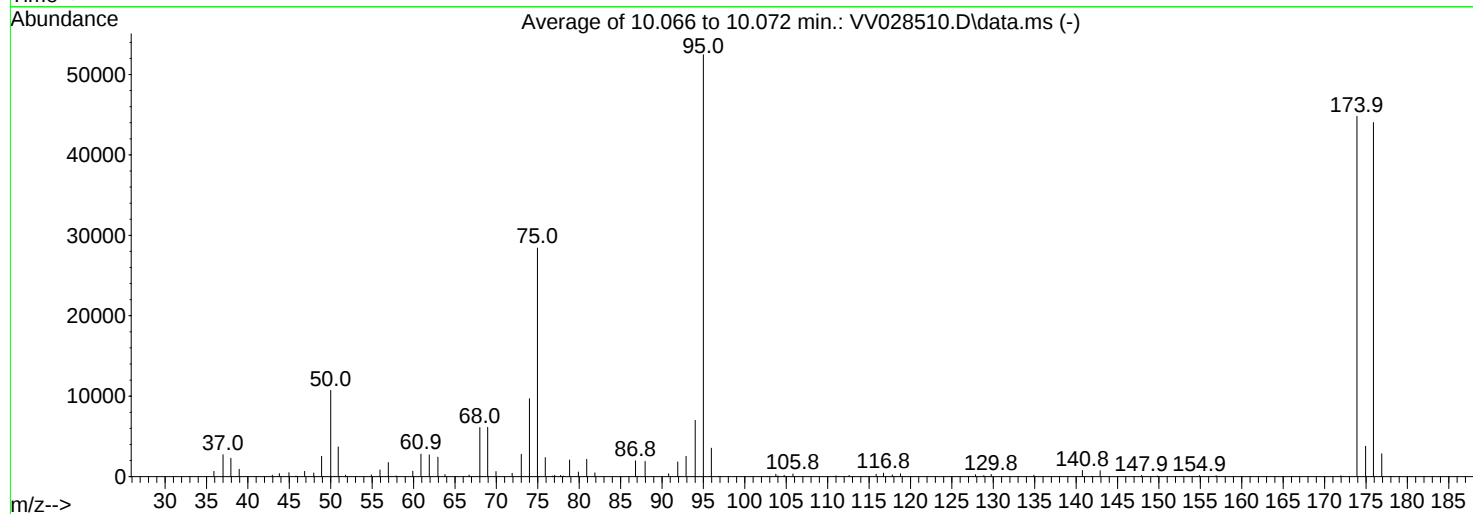


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101122\
Data File : VV028510.D
Acq On : 11 Oct 2022 09:45
Operator : SY/MD
Sample : BFB328
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB328

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Title : VOC Analysis
Last Update : Thu Oct 13 02:58:16 2022

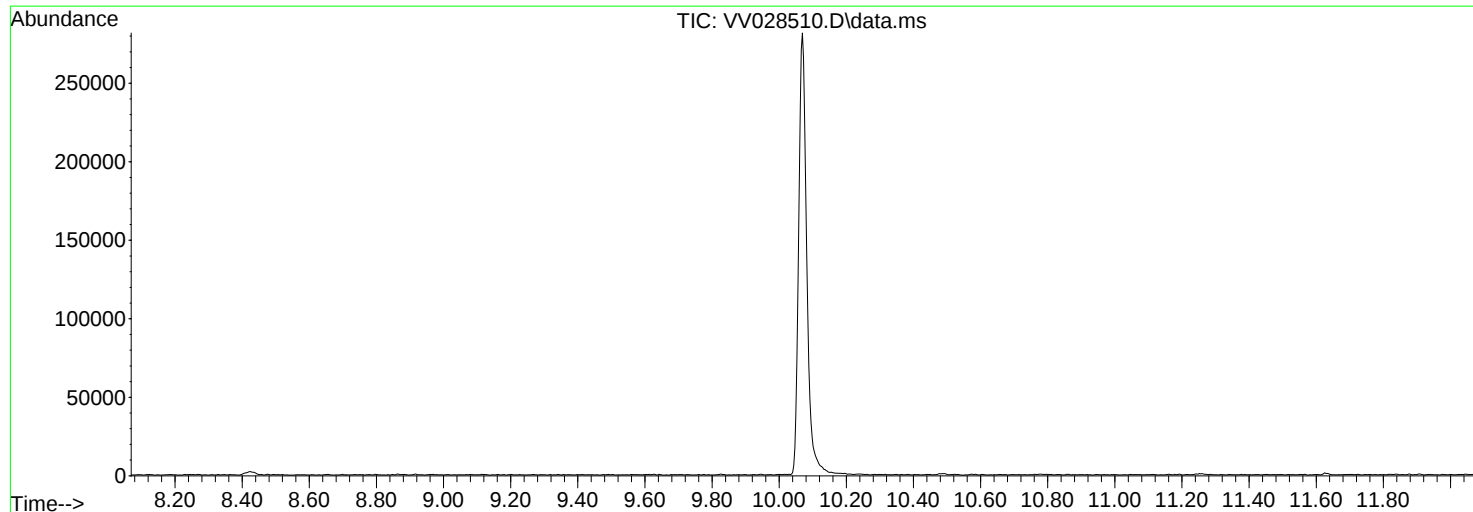

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	10721	PASS
75	95	30	80	54.2	28435	PASS
95	95	100	100	100.0	52459	PASS
96	95	5	9	6.7	3535	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.4	44813	PASS
175	174	5	9	8.4	3778	PASS
176	174	95	105	98.2	44027	PASS
177	176	5	10	6.5	2846	PASS

m/z	Abundance
39.80	319.0
41.10	129.0
42.70	107.0
43.80	327.0
67.70	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328

m/z	Abundance
35.90	615.0
37.00	2786.0
38.00	2410.0
39.00	934.0
39.90	335.0
40.90	108.0
42.90	199.0
43.90	757.0
44.90	450.0
46.80	619.0
48.00	470.0
48.90	2635.0
50.00	10756.0
50.90	3718.0
51.80	214.0
54.90	183.0
55.90	847.0
56.90	1770.0
57.90	167.0
59.90	608.0
60.90	2782.0
61.90	2687.0
63.00	2341.0
63.80	267.0
66.70	207.0
68.00	6165.0
69.00	6182.0
70.00	615.0
71.90	376.0
73.00	2759.0
74.00	9664.0
74.90	29192.0
75.90	2458.0
76.80	209.0
78.80	2013.0
79.90	580.0
80.90	2098.0
81.90	465.0
86.80	1920.0
87.90	1899.0
90.80	334.0
91.90	1811.0
92.90	2516.0
94.00	6875.0
95.00	51576.0
95.90	3814.0
96.80	110.0
103.80	317.0
104.80	168.0
105.80	357.0
111.00	128.0
112.60	135.0
115.80	261.0
116.70	436.0
117.80	189.0
118.90	303.0
127.80	239.0
128.90	118.0
129.80	302.0
134.80	168.0
140.70	737.0
141.90	121.0
142.90	750.0
147.90	128.0
149.80	126.0
154.90	129.0
156.90	108.0
173.90	44296.0
174.90	3771.0
175.90	42600.0
176.90	2784.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328

m/z	Abundance
35.90	666.0
37.00	2798.0
37.90	2337.0
39.00	924.0
39.90	282.0
40.90	107.0
42.90	189.0
43.90	690.0
45.00	513.0
45.80	109.0
46.90	674.0
48.00	483.0
48.90	2594.0
50.00	11101.0
50.90	3885.0
51.80	171.0
54.90	229.0
56.00	855.0
56.90	1792.0
57.90	121.0
59.90	680.0
60.90	2929.0
61.90	2753.0
63.00	2541.0
63.80	245.0
66.70	205.0
68.00	6319.0
68.90	6231.0
70.00	651.0
71.90	418.0
73.00	2855.0
74.00	9906.0
75.00	29048.0
75.90	2413.0
77.10	243.0
77.80	224.0
78.10	236.0
78.80	2103.0
79.90	585.0
80.90	2233.0
81.90	480.0
86.80	1995.0
87.90	1965.0
90.80	373.0
91.90	1864.0
92.90	2619.0
94.00	7305.0
95.00	54072.0
96.00	3599.0
102.70	108.0
103.70	301.0
104.70	174.0
105.80	350.0
111.00	118.0
112.60	173.0
115.80	297.0
116.70	450.0
117.80	227.0
118.80	353.0
127.90	232.0
128.90	138.0
129.80	283.0
134.90	178.0
140.70	782.0
142.90	767.0
147.90	155.0
149.80	115.0
154.90	133.0
156.90	107.0
171.90	149.0
173.90	46360.0
174.90	3883.0
175.90	45480.0
176.90	2991.0
178.00	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328

m/z	Abundance
35.90	669.0
37.00	2577.0
37.90	2088.0
38.90	865.0
40.00	266.0
43.00	146.0
43.80	655.0
45.00	509.0
45.80	101.0
46.90	628.0
47.90	403.0
48.90	2325.0
50.00	10306.0
50.90	3461.0
51.80	137.0
54.90	235.0
56.00	805.0
57.00	1657.0
59.90	723.0
60.90	2660.0
61.90	2625.0
62.90	2373.0
63.80	216.0
66.70	171.0
68.00	5820.0
68.90	5935.0
69.90	593.0
71.90	428.0
73.00	2715.0
74.00	9475.0
75.00	27064.0
75.90	2206.0
77.00	280.0
77.70	241.0
78.90	2041.0
79.90	511.0
80.90	2096.0
81.90	440.0
86.80	1997.0
88.00	1787.0
90.80	364.0
91.90	1808.0
92.90	2408.0
94.00	6816.0
95.00	51728.0
96.00	3191.0
103.70	258.0
104.00	252.0
104.70	152.0
105.80	297.0
112.60	123.0
115.90	309.0
116.80	399.0
117.80	219.0
118.70	368.0
127.90	224.0
128.80	160.0
129.70	228.0
135.00	152.0
140.80	757.0
142.90	694.0
147.90	176.0
154.90	138.0
156.90	111.0
172.00	127.0
173.90	43784.0
175.00	3679.0
175.90	44000.0
176.90	2762.0

Instrument :
MSVOA_V
ClientSampleId :
BFB328