

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
 Data File : VV032387.D
 Acq On : 11 Oct 2023 12:45
 Operator : SY/MD
 Sample : 04851-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B11

Quant Time: Oct 12 03:04:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 12 02:54:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	102370	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	115730	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	51897	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	35995	4.323	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.400%
7) Chloroethane-d5	1.532	69	30481	4.510	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.200%
11) 1,1-Dichloroethene-d2	2.059	65	13620	3.879	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.600%
20) 2-Butanone-d5	3.805	46	76515	36.330	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	72.660%
24) Chloroform-d	4.256	84	61383	4.179	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.600%
26) 1,2-Dichloroethane-d4	4.950	65	29595	4.254	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.000%
32) Benzene-d6	4.966	84	118106	3.468	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	69.400%#
36) 1,2-Dichloropropane-d6	5.995	67	38559	3.418	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	68.400%
41) Toluene-d8	7.249	98	109507	3.517	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	70.400%
43) trans-1,3-Dichloroprop...	7.561	79	13699	3.426	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.600%
46) 2-Hexanone-d5	8.030	63	68592	36.464	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	72.920%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	30389	3.851	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	77.000%
66) 1,2-Dichlorobenzene-d4	11.567	152	41566	4.316	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	86.400%
Target Compounds			Qvalue			
25) Chloroform	4.284	83	14648	0.923	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032387.D
Acq On : 11 Oct 2023 12:45
Operator : SY/MD
Sample : 04851-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B11

Quant Time: Oct 12 03:04:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 12 02:54:58 2023
Response via : Initial Calibration

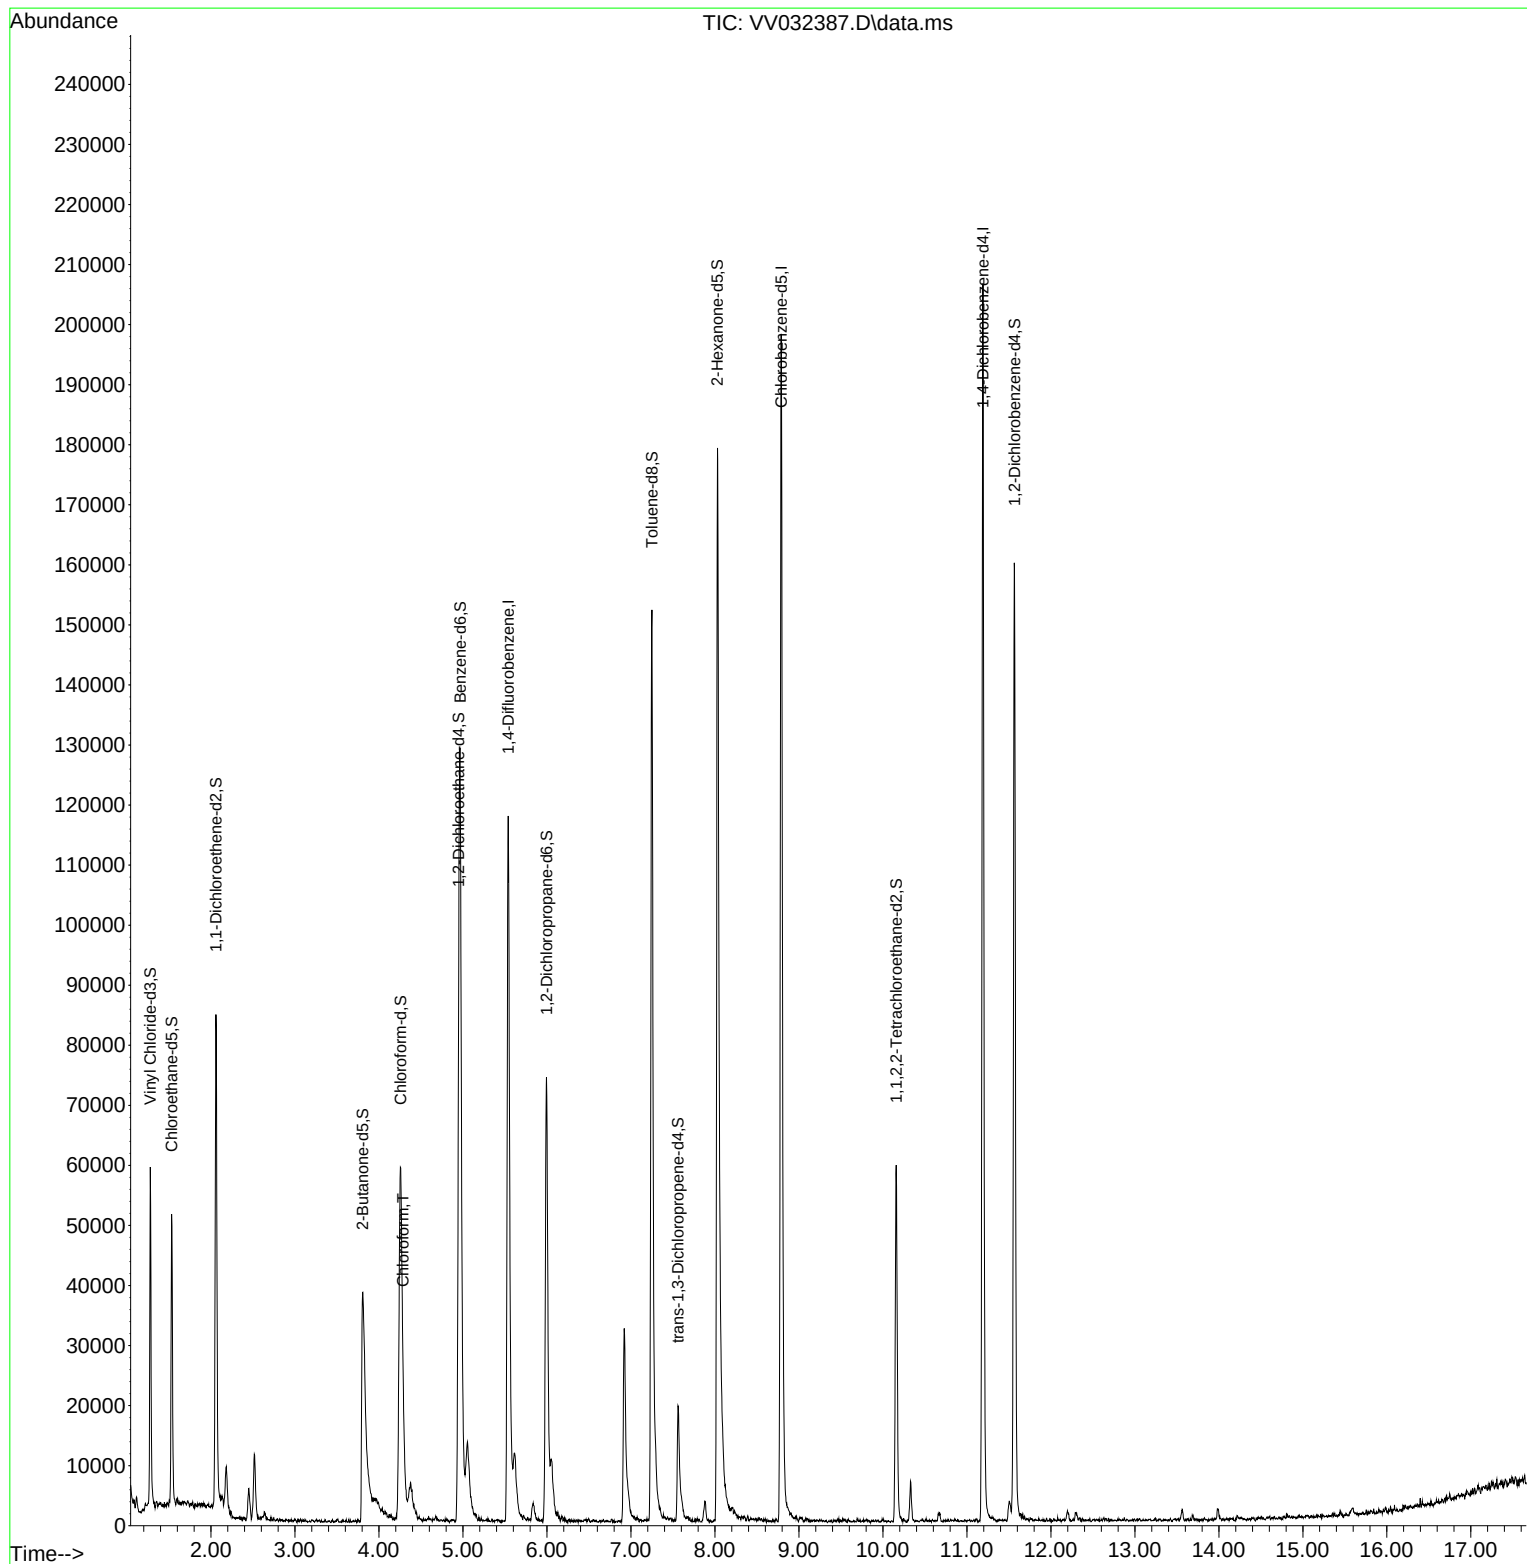

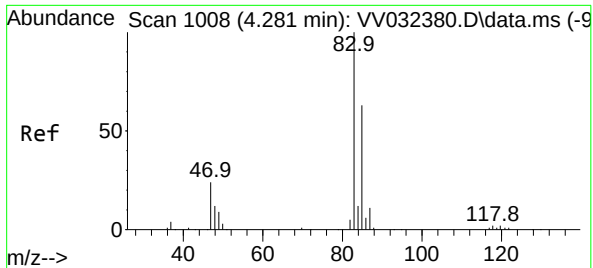

#25
 Chloroform
 Concen: 0.923 ug/L
 RT: 4.284 min Scan# 10
 Delta R.T. 0.003 min
 Lab File: VV032387.D
 Acq: 11 Oct 2023 12:45

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B11

Tgt Ion: 83 Resp: 14648
 Ion Ratio Lower Upper
 83 100
 85 64.9 45.4 84.4

