

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
 Data File : VV032402.D
 Acq On : 11 Oct 2023 18:44
 Operator : SY/MD
 Sample : 04826-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCJV0

Quant Time: Oct 12 03:07:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 12 02:54:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	105142	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	114065	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	51850	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	33266	3.890	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.800%
7) Chloroethane-d5	1.532	69	28967	4.173	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.400%
11) 1,1-Dichloroethene-d2	2.060	65	14182	3.933	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.600%
20) 2-Butanone-d5	3.802	46	84456	39.043	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	78.080%
24) Chloroform-d	4.256	84	65055	4.313	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.200%
26) 1,2-Dichloroethane-d4	4.947	65	30720	4.299	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.000%
32) Benzene-d6	4.966	84	116120	3.460	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	69.200%#
36) 1,2-Dichloropropane-d6	5.992	67	39953	3.593	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	71.800%
41) Toluene-d8	7.246	98	105788	3.447	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	69.000%#
43) trans-1,3-Dichloroprop...	7.561	79	13380	3.395	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.000%
46) 2-Hexanone-d5	8.030	63	71061	38.328	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.660%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	30788	3.958	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	79.200%
66) 1,2-Dichlorobenzene-d4	11.564	152	41157	4.278	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	85.600%
Target Compounds						
					Qvalue	
13) Acetone	2.130	43	5363	3.217	ug/L	96
22) cis-1,2-Dichloroethene	3.822	96	1771	0.186	ug/L	78
25) Chloroform	4.281	83	73321	4.498	ug/L	99
33) Benzene	5.018	78	24566	0.612	ug/L	100
34) Trichloroethene	5.834	95	2383633	217.423	ug/L	98
38) Bromodichloromethane	6.442	83	9488	0.743	ug/L	99
42) Toluene	7.326	91	15608	0.365	ug/L	98
47) Tetrachloroethene	7.908	164	4920	0.592	ug/L	96
49) Dibromochloromethane	8.182	129	1814	0.230	ug/L	96
52) Ethylbenzene	8.956	91	2531	0.053	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032402.D
Acq On : 11 Oct 2023 18:44
Operator : SY/MD
Sample : 04826-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJV0

Quant Time: Oct 12 03:07:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 12 02:54:58 2023
Response via : Initial Calibration

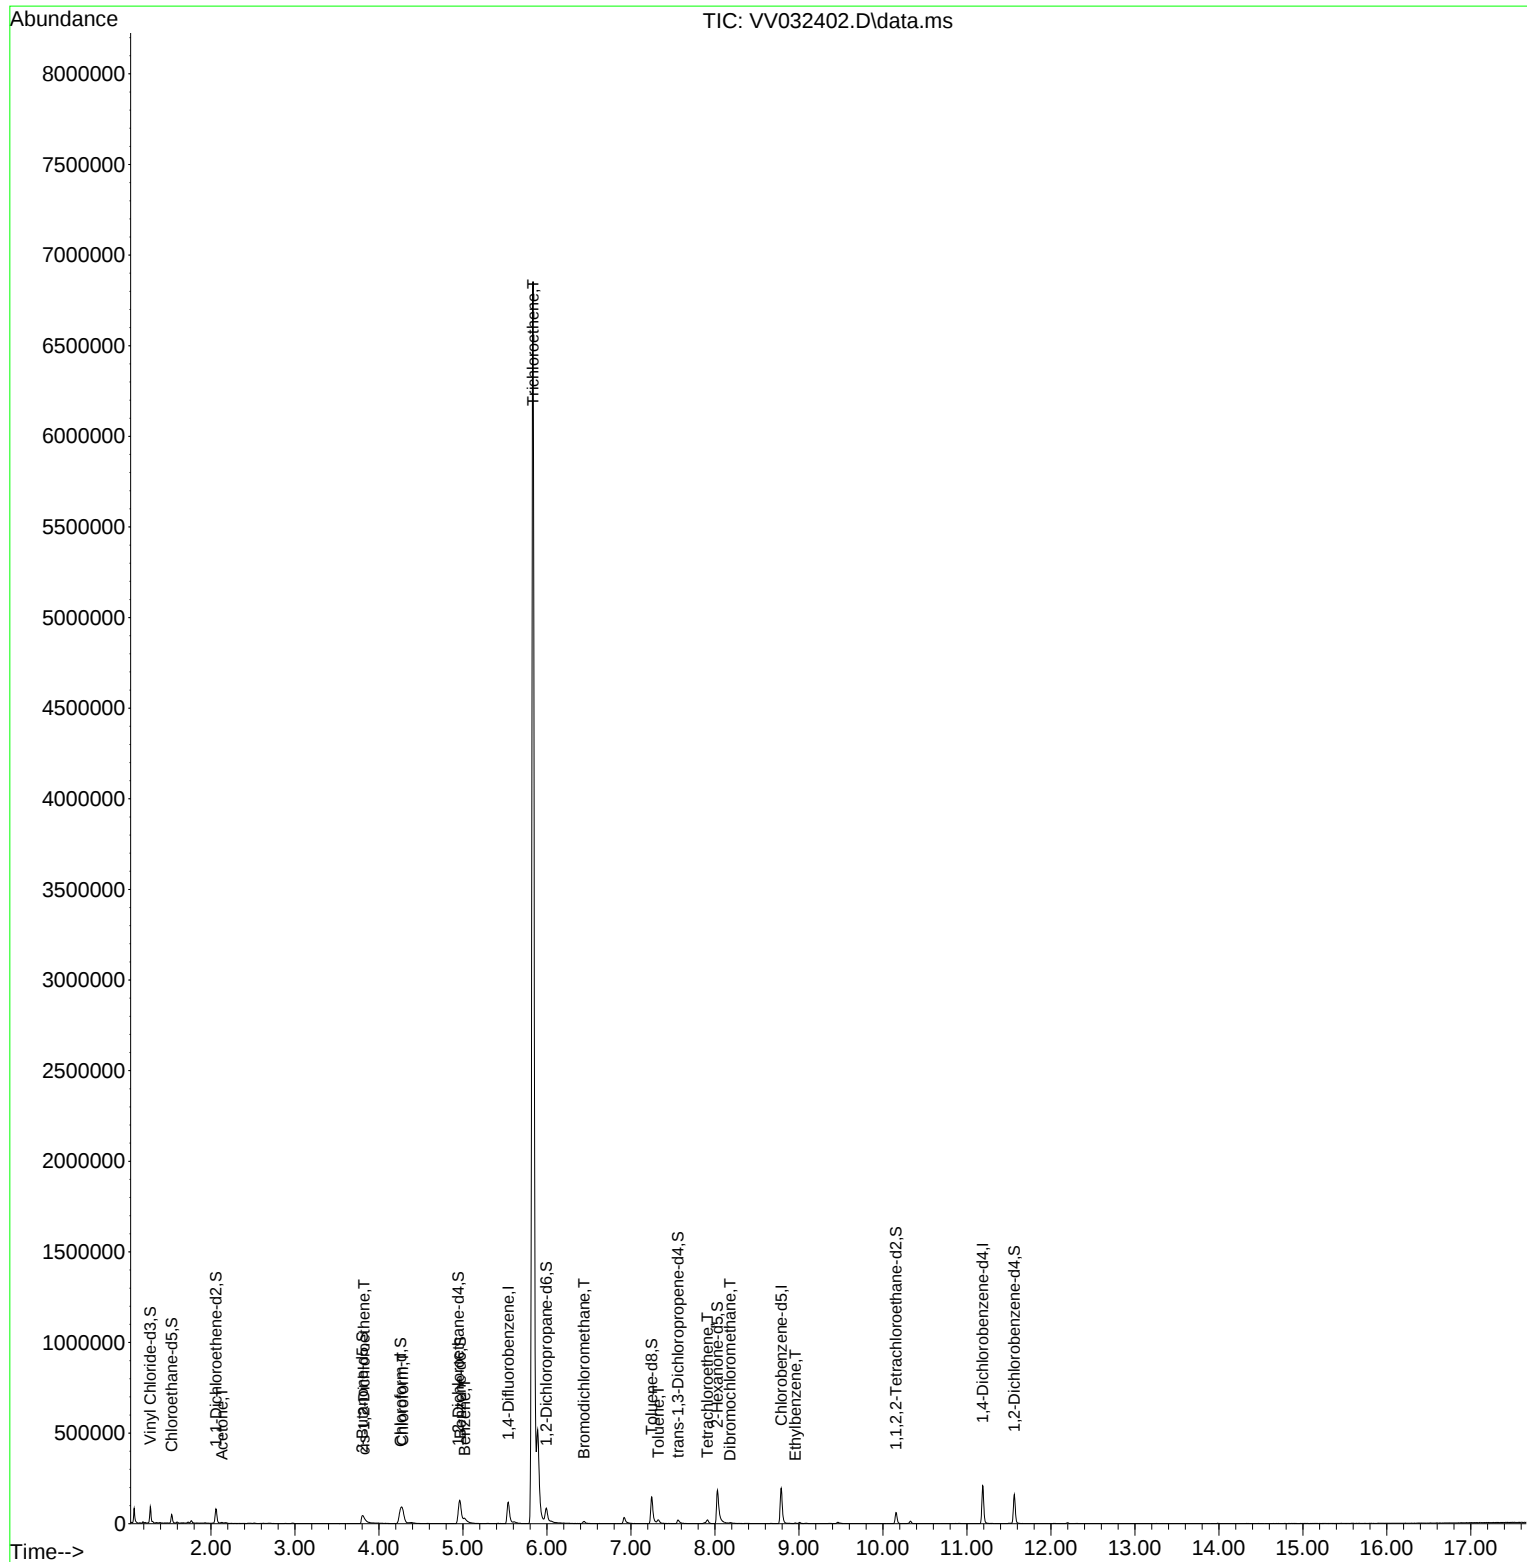

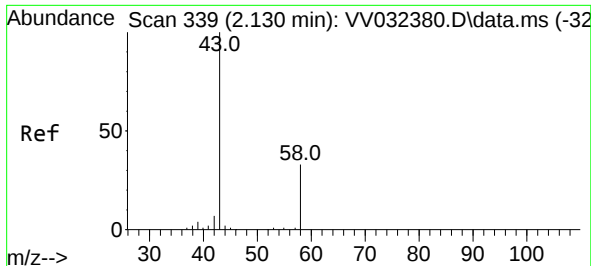

#13

Acetone

Concen: 3.217 ug/L

RT: 2.130 min Scan# 31

Delta R.T. 0.000 min

Lab File: VV032402.D

Acq: 11 Oct 2023 18:44

Instrument :

MSVOA_V

ClientSampleId :





DCJV0

Tgt Ion: 43 Resp: 5363

Ion Ratio Lower Upper

43 100

58 35.0 0.0 66.0

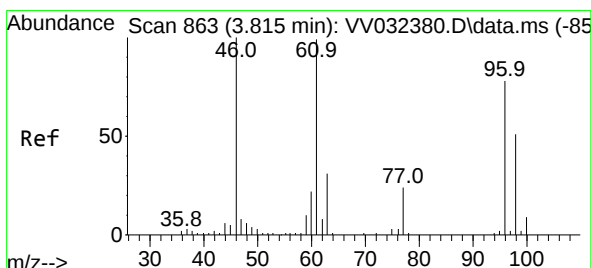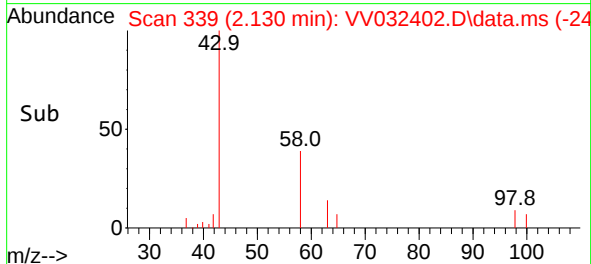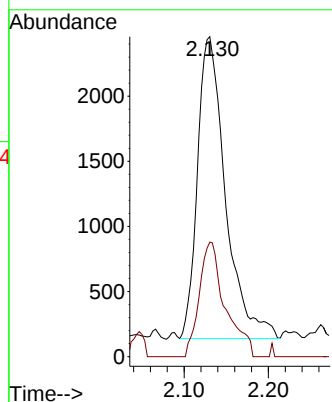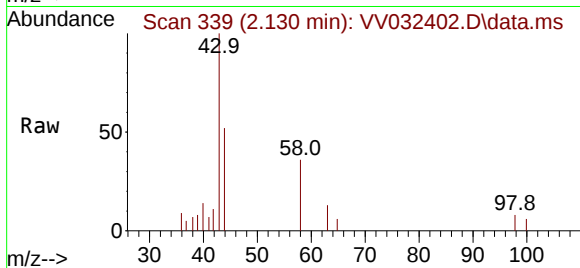

#22

cis-1,2-Dichloroethene

Concen: 0.186 ug/L

RT: 3.822 min Scan# 865

Delta R.T. 0.007 min

Lab File: VV032402.D

Acq: 11 Oct 2023 18:44




Tgt Ion: 96 Resp: 1771


Ion Ratio Lower Upper

96 100

61 158.2 85.8 159.4

98 64.7 44.0 81.6

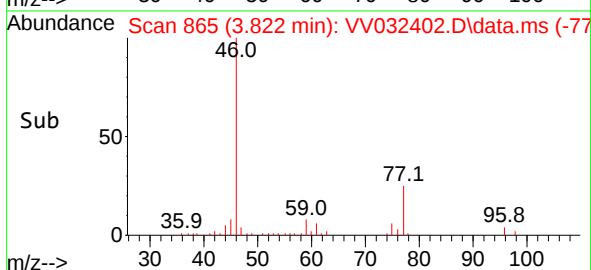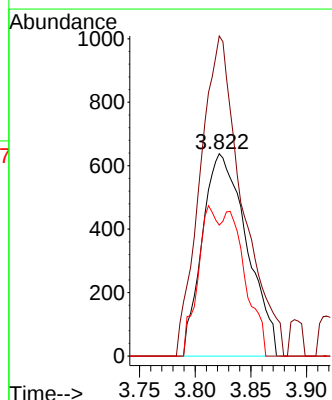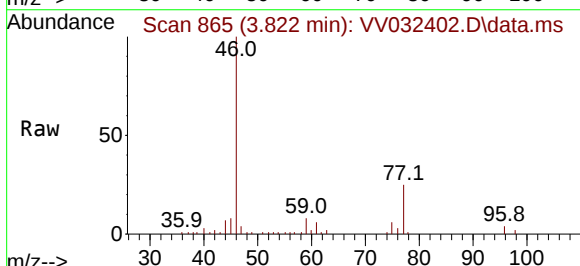

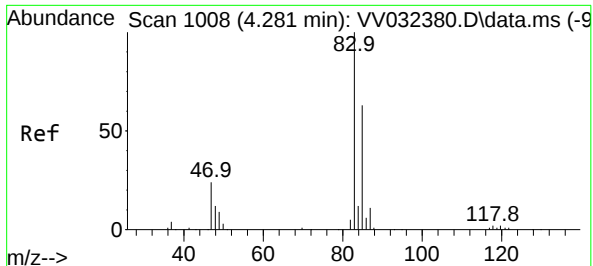

#25

Chloroform

Concen: 4.498 ug/L

RT: 4.281 min Scan# 1008

Delta R.T. 0.000 min

Lab File: VV032402.D

Acq: 11 Oct 2023 18:44

Instrument :

MSVOA_V

ClientSampleId :





DCJV0

Tgt Ion: 83 Resp: 73321

Ion Ratio Lower Upper

83 100

85 64.0 45.4 84.4

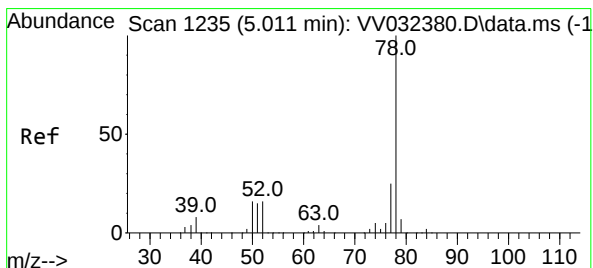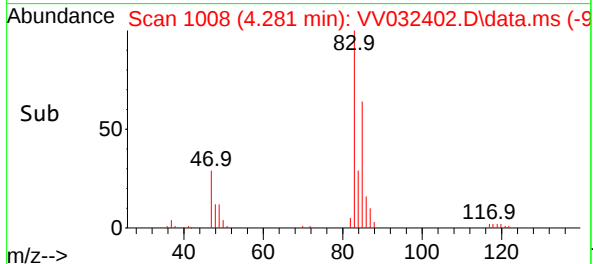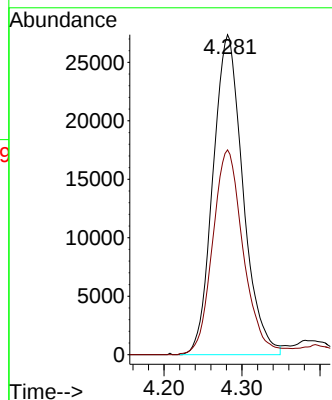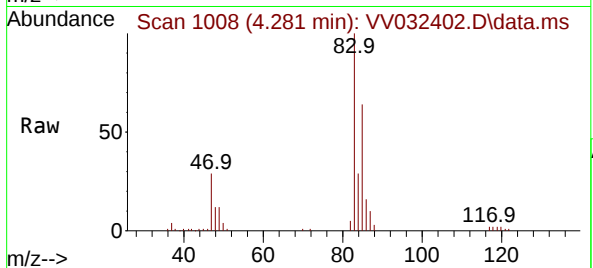

#33

Benzene

Concen: 0.612 ug/L




RT: 5.018 min Scan# 1237


Delta R.T. 0.007 min

Lab File: VV032402.D

Acq: 11 Oct 2023 18:44

Tgt Ion: 78 Resp: 24566

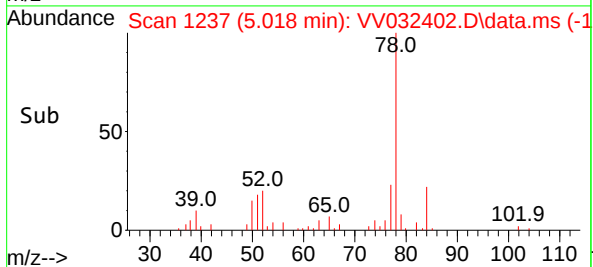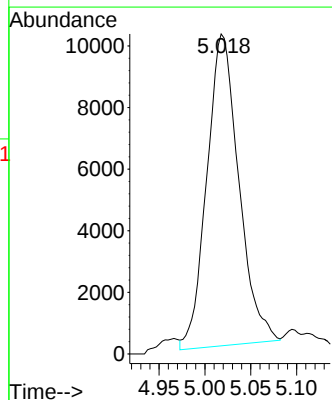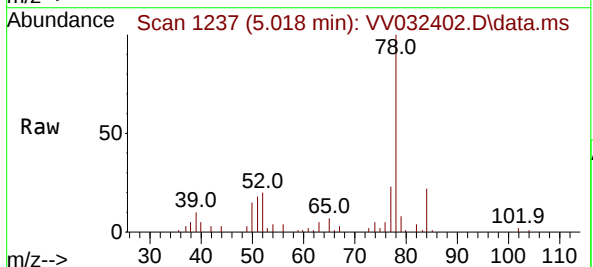




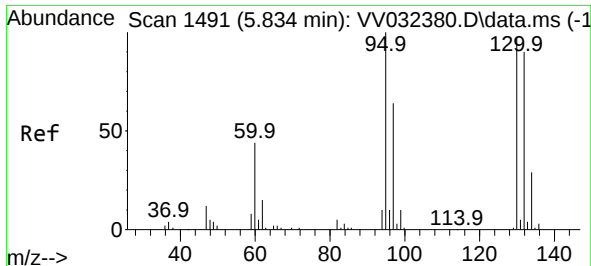


#34
Trichloroethene
Concen: 217.423 ug/L
RT: 5.834 min Scan# 1491
Delta R.T. 0.000 min
Lab File: VV032402.D
Acq: 11 Oct 2023 18:44

Instrument :
MSVOA_V
ClientSampleId :
DCJV0

Tgt Ion: 95 Resp: 2383633




Ion	Ratio	Lower	Upper
95	100		
97	65.3	45.7	84.9
132	95.3	70.3	130.5
130	99.4	69.6	129.2

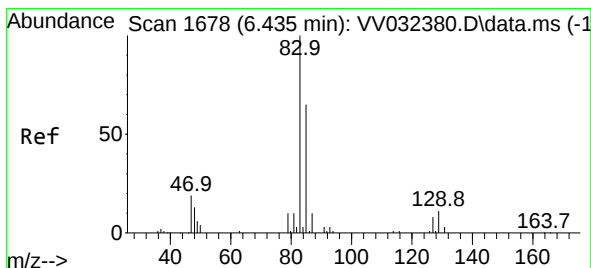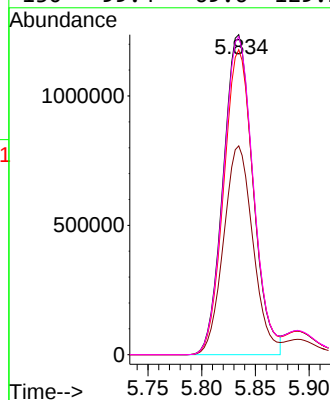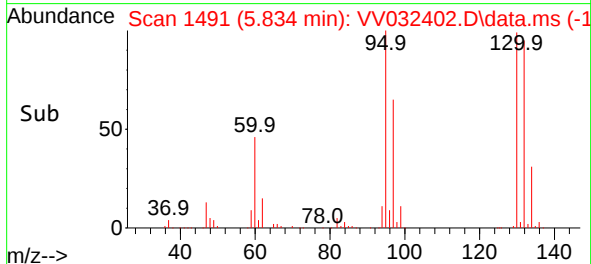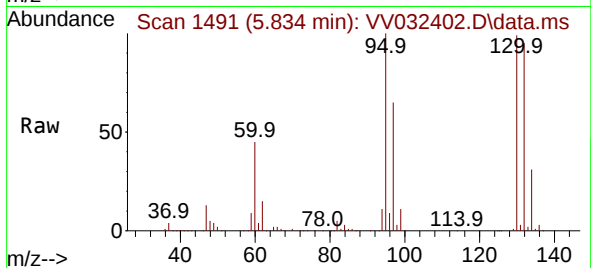


#38
Bromodichloromethane
Concen: 0.743 ug/L
RT: 6.442 min Scan# 1680
Delta R.T. 0.007 min
Lab File: VV032402.D
Acq: 11 Oct 2023 18:44

Tgt Ion: 83 Resp: 9488

Ion	Ratio	Lower	Upper
83	100		
85	63.0	44.9	83.3
127	9.2	6.9	10.3

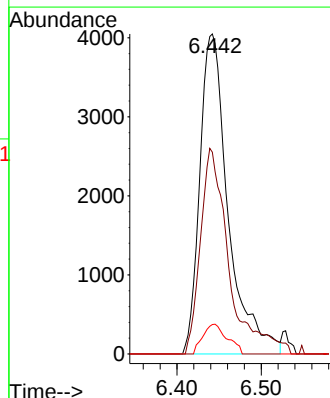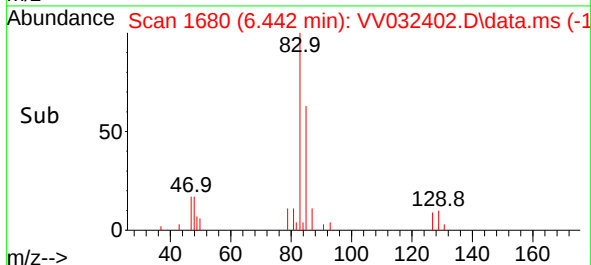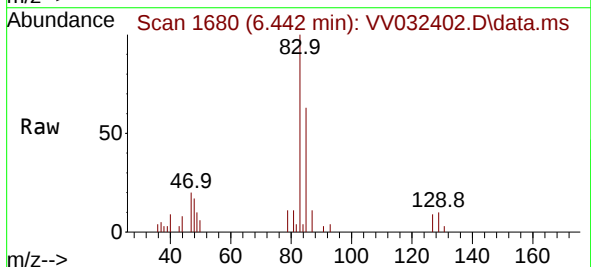

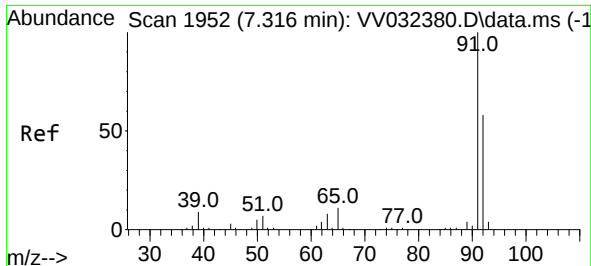

#42

Toluene

Concen: 0.365 ug/L

RT: 7.326 min Scan# 1955

Delta R.T. 0.010 min

Lab File: VV032402.D

Acq: 11 Oct 2023 18:44

Instrument :

MSVOA_V

ClientSampleId :





DCJV0

Tgt Ion: 91 Resp: 15608

Ion Ratio Lower Upper

91 100

92 57.1 40.8 75.8

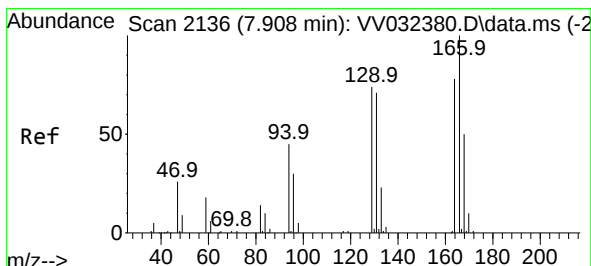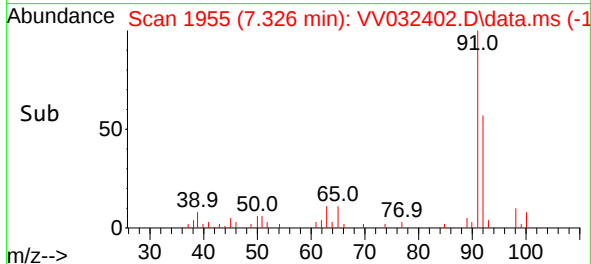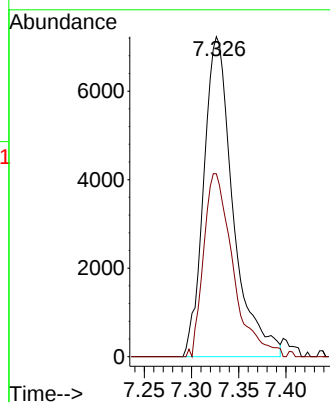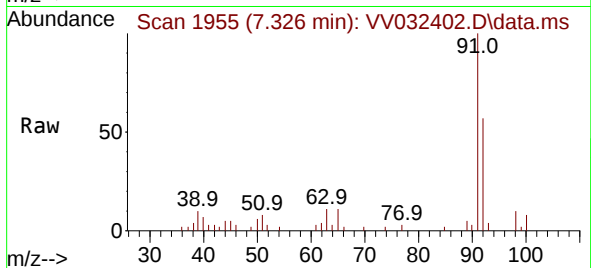

#47

Tetrachloroethene

Concen: 0.592 ug/L

RT: 7.908 min Scan# 2136

Delta R.T. 0.000 min

Lab File: VV032402.D

Acq: 11 Oct 2023 18:44

Tgt Ion:164 Resp: 4920




Ion Ratio Lower Upper


164 100

129 93.5 66.4 123.4

131 96.7 63.7 118.3

166 129.6 87.9 163.3

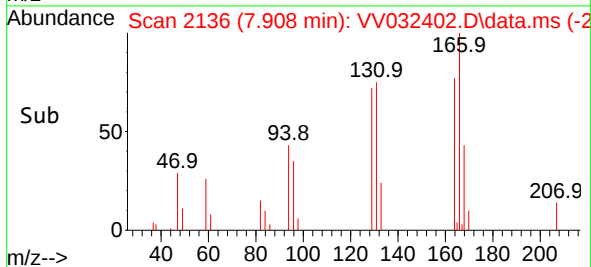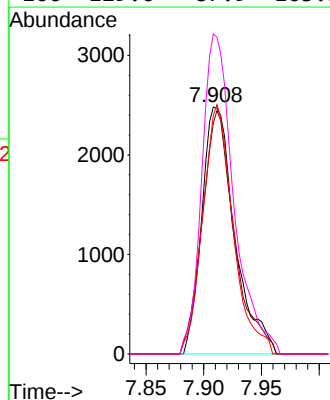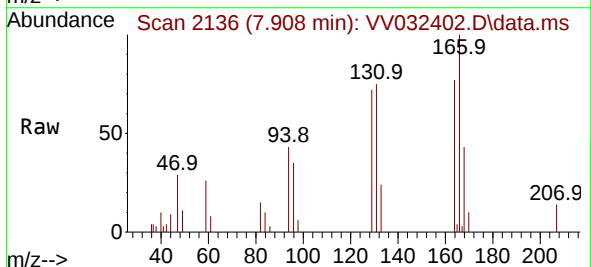

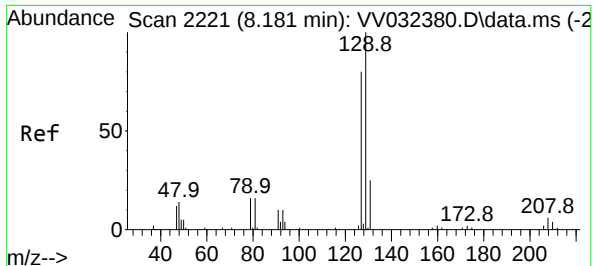

#49

Dibromochloromethane

Concen: 0.230 ug/L

RT: 8.182 min Scan# 21

Delta R.T. 0.000 min

Lab File: VV032402.D

Acq: 11 Oct 2023 18:44

Instrument :

MSVOA_V

ClientSampleId :





DCJV0

Tgt Ion:129 Resp: 1814

Ion Ratio Lower Upper

129 100

127 85.6 57.2 106.2

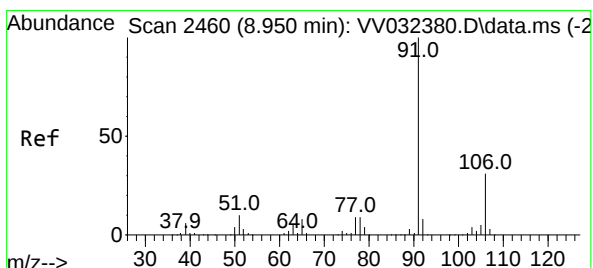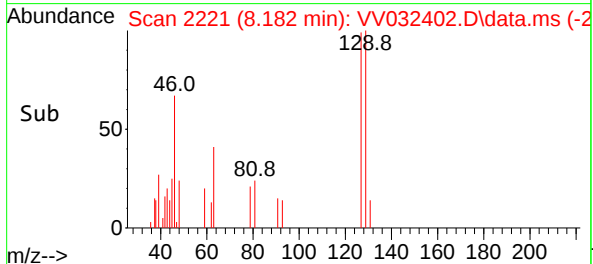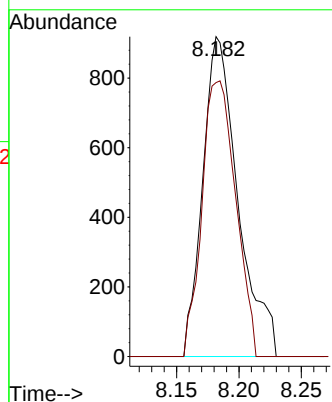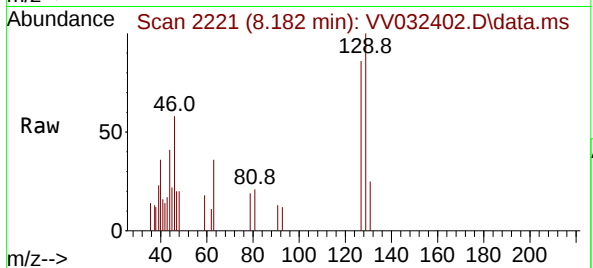

#52

Ethylbenzene

Concen: 0.053 ug/L

RT: 8.956 min Scan# 2462

Delta R.T. 0.007 min

Lab File: VV032402.D

Acq: 11 Oct 2023 18:44

Tgt Ion: 91 Resp: 2531

Ion Ratio Lower Upper

91 100

106 23.2 21.3 39.5

