

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
 Data File : VV032381.D
 Acq On : 11 Oct 2023 10:09
 Operator : SY/MD
 Sample : VV1011WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK369

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032381.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	16	21	33	rVB	5305	7969	1.95%	0.248%
2	1.278	66	74	87	rBV	60669	65206	15.99%	2.026%
3	1.532	145	153	168	rVB	52136	62177	15.25%	1.932%
4	2.060	307	317	334	rBV	88543	130636	32.04%	4.059%
5	2.175	345	353	365	rVB2	6694	13941	3.42%	0.433%
6	3.818	854	864	897	rBV2	33807	136760	33.55%	4.249%
7	4.253	982	999	1021	rBV	59422	156216	38.32%	4.853%
8	4.963	1204	1220	1238	rBV3	136093	351586	86.24%	10.923%
9	5.539	1388	1399	1415	rBV	113756	237727	58.31%	7.386%
10	5.606	1415	1420	1436	rVB2	8962	22651	5.56%	0.704%
11	5.838	1483	1492	1497	rBV5	3044	5455	1.34%	0.169%
12	5.992	1528	1540	1555	rBV2	79102	171829	42.15%	5.338%
13	6.921	1819	1829	1855	rBV	34683	78843	19.34%	2.450%
14	7.249	1919	1931	1964	rBV	159704	313929	77.00%	9.753%
15	7.561	2018	2028	2052	rBV2	20638	44196	10.84%	1.373%
16	8.031	2165	2174	2211	rBV	188492	407685	100.00%	12.666%
17	8.789	2398	2410	2434	rBV	191054	331264	81.25%	10.292%
18	10.159	2825	2836	2849	rBV	64264	104987	25.75%	3.262%
19	11.188	3146	3156	3180	rBV	189696	305277	74.88%	9.484%
20	11.564	3262	3273	3290	rBV	165106	265743	65.18%	8.256%
21	17.159	5010	5013	5020	rVB	6731	4653	1.14%	0.145%




Sum of corrected areas: 3218730

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032381.D
Acq On : 11 Oct 2023 10:09
Operator : SY/MD
Sample : VV1011WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK369

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

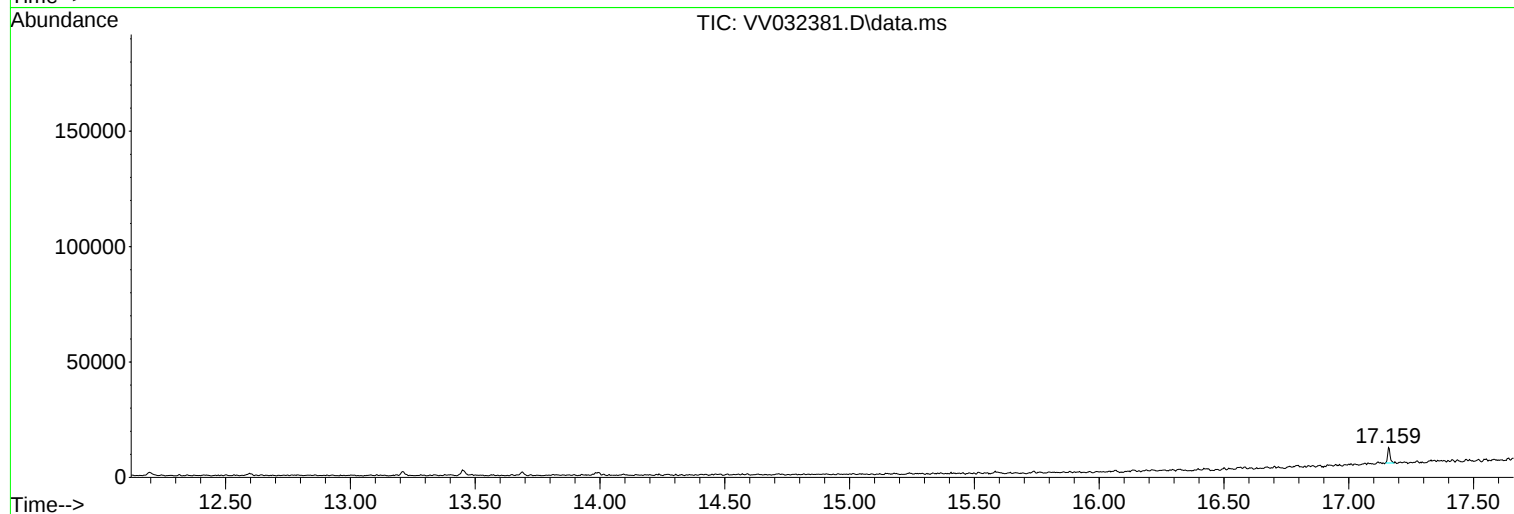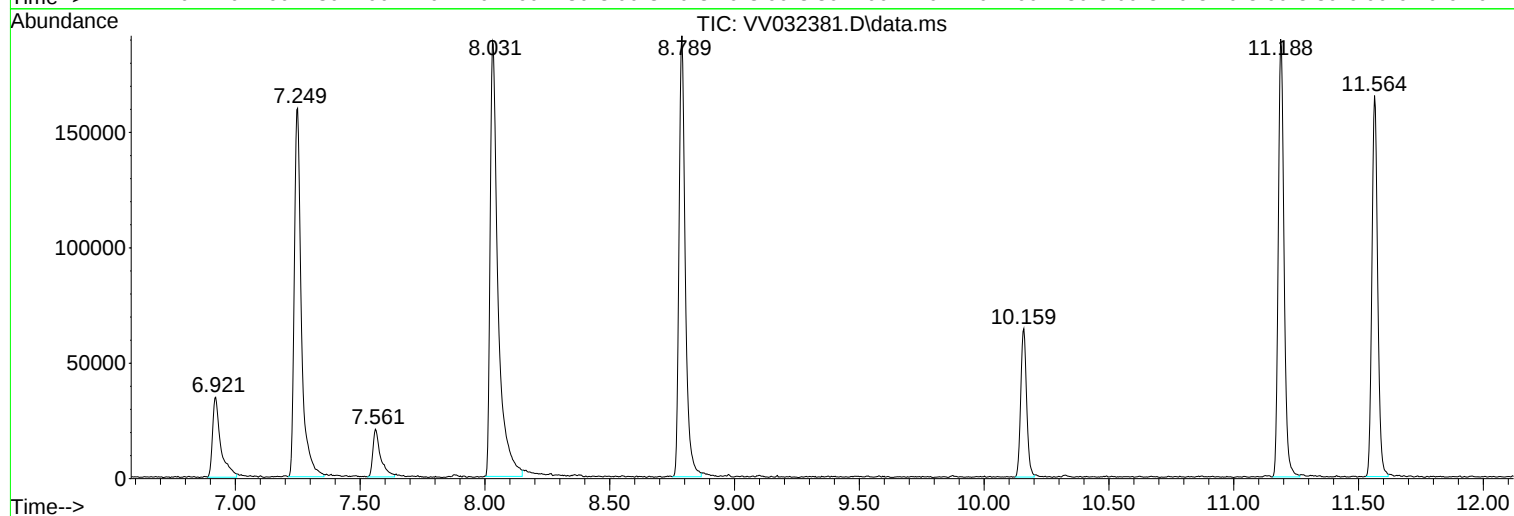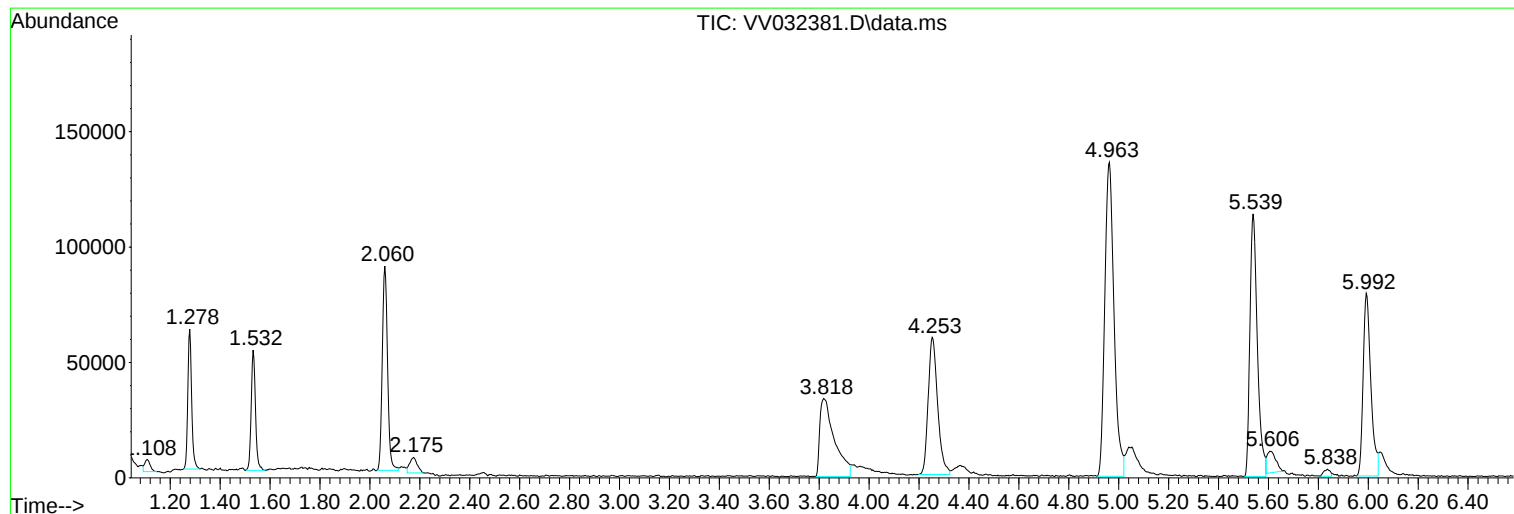

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032381.D
Acq On : 11 Oct 2023 10:09
Operator : SY/MD
Sample : VV1011WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK369

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032381.D
Acq On : 11 Oct 2023 10:09
Operator : SY/MD
Sample : VV1011WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK369

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc