

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
 Data File : VV032383.D
 Acq On : 11 Oct 2023 11:07
 Operator : SY/MD
 Sample : 04708-11DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCJT3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032383.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	19	rBV	15983	13998	3.40%	0.374%
2	1.278	65	74	93	rBV	67522	76050	18.46%	2.030%
3	1.532	146	153	167	rBV	51117	59868	14.53%	1.598%
4	2.060	306	317	330	rBV	89043	131663	31.96%	3.515%
5	2.179	346	354	367	rVB4	8016	15986	3.88%	0.427%
6	2.449	424	438	453	rVB	8301	15039	3.65%	0.401%
7	3.809	848	861	897	rBV2	50708	181144	43.97%	4.835%
8	4.256	983	1000	1024	rBV2	61859	180785	43.88%	4.826%
9	4.963	1205	1220	1239	rBV3	135840	353382	85.77%	9.433%
10	5.539	1387	1399	1415	rBV2	121184	253054	61.42%	6.755%
11	5.834	1478	1491	1506	rBV	186891	386699	93.86%	10.323%
12	5.995	1528	1541	1554	rBV2	76750	162647	39.48%	4.342%
13	6.921	1819	1829	1855	rBV2	33639	77603	18.84%	2.072%
14	7.246	1920	1930	1964	rBV	161615	316856	76.91%	8.458%
15	7.561	2018	2028	2046	rBV	21357	43687	10.60%	1.166%
16	8.030	2164	2174	2204	rBV	194149	411990	100.00%	10.998%
17	8.789	2399	2410	2434	rBV	200203	351607	85.34%	9.386%
18	10.159	2824	2836	2858	rBV	64655	107378	26.06%	2.866%
19	10.329	2875	2889	2901	rBV4	5515	9160	2.22%	0.245%
20	11.188	3146	3156	3176	rBV	201039	325781	79.07%	8.696%
21	11.564	3262	3273	3290	rBV	170880	271758	65.96%	7.254%




Sum of corrected areas: 3746135

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032383.D
Acq On : 11 Oct 2023 11:07
Operator : SY/MD
Sample : 04708-11DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJT3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

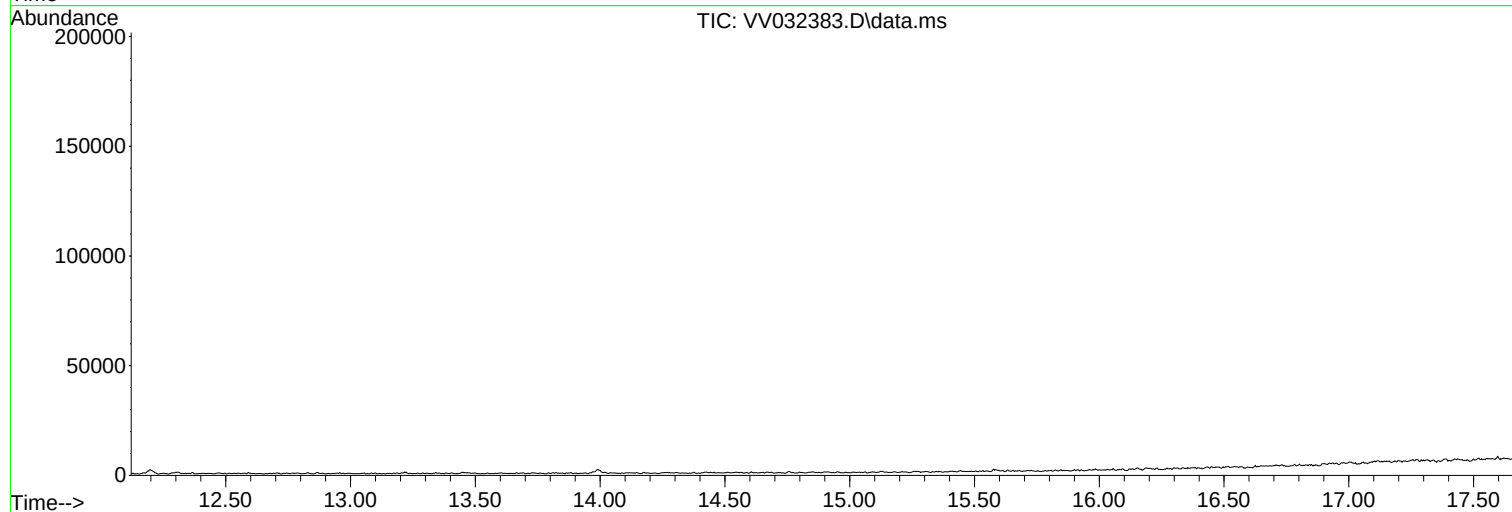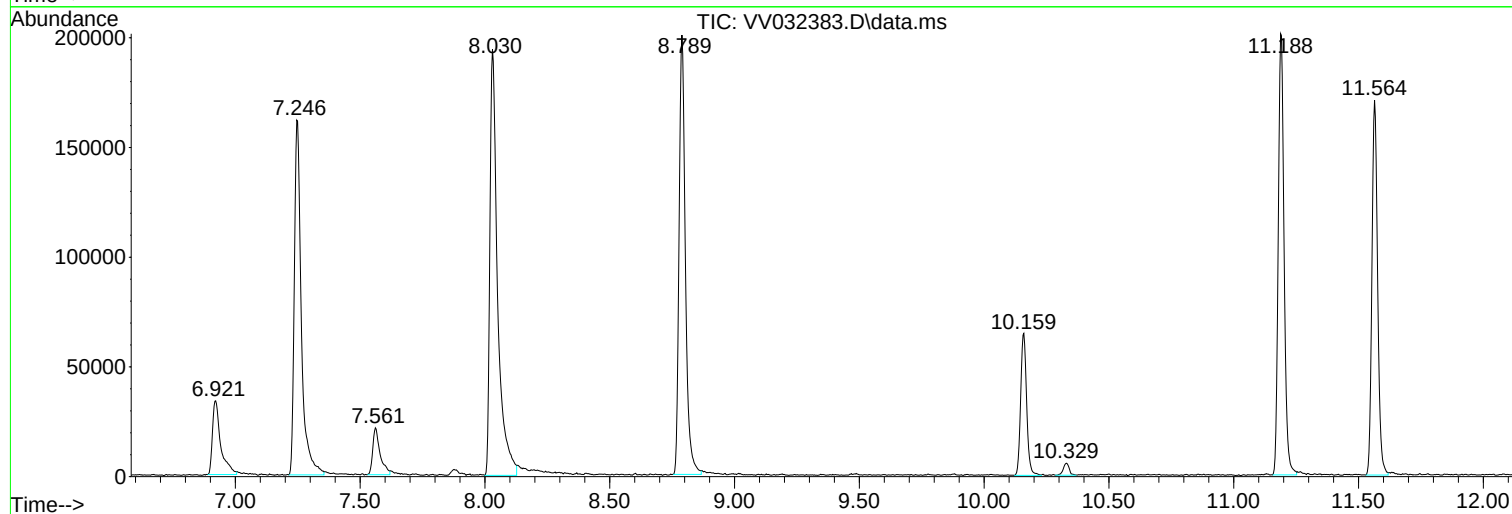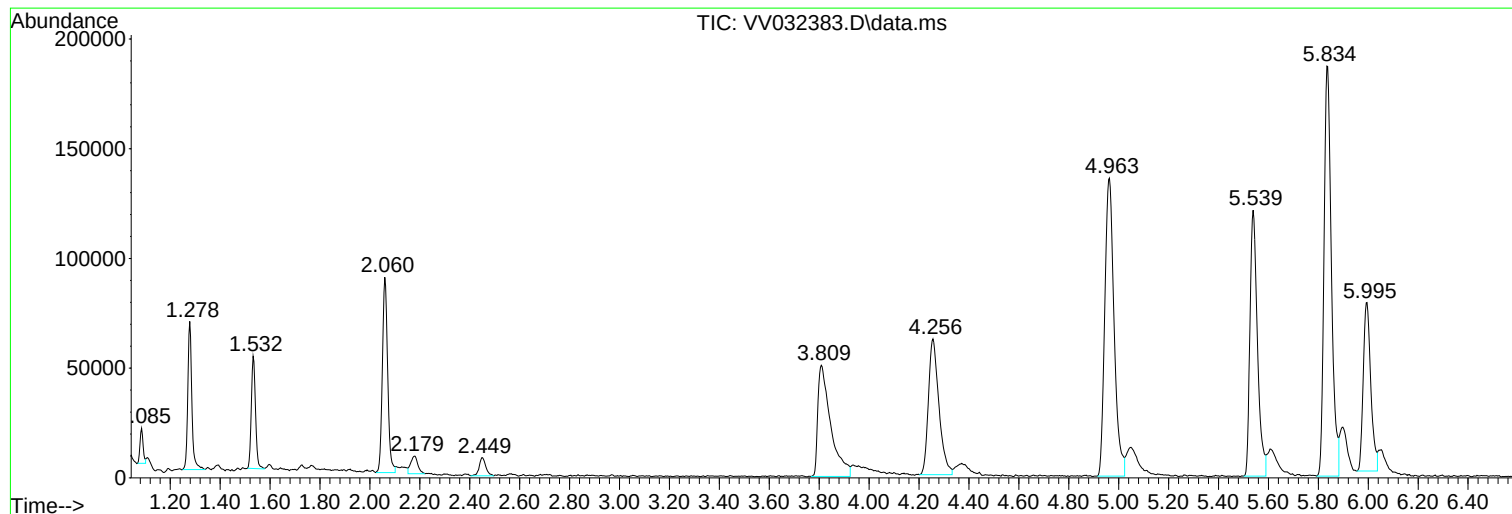

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032383.D
Acq On : 11 Oct 2023 11:07
Operator : SY/MD
Sample : 04708-11DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJT3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032383.D
Acq On : 11 Oct 2023 11:07
Operator : SY/MD
Sample : 04708-11DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJT3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc