

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
 Data File : VV032386.D
 Acq On : 11 Oct 2023 12:20
 Operator : SY/MD
 Sample : 04851-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032386.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	60309	65055	15.66%	1.970%
2	1.532	145	153	168	rBV	50763	61295	14.76%	1.856%
3	2.060	307	317	332	rBV	85055	124093	29.88%	3.757%
4	2.175	348	353	370	rVB3	7629	15471	3.72%	0.468%
5	2.449	429	438	448	rBV6	2955	5212	1.25%	0.158%
6	2.516	450	459	473	rVB3	6504	11951	2.88%	0.362%
7	3.812	850	862	893	rBV	36717	131782	31.73%	3.990%
8	4.259	983	1001	1027	rBV4	76461	241408	58.12%	7.309%
9	4.963	1205	1220	1239	rBV2	136608	349263	84.09%	10.574%
10	5.539	1388	1399	1416	rBV	117494	247240	59.53%	7.485%
11	5.995	1528	1541	1556	rBV	75337	165303	39.80%	5.005%
12	6.921	1818	1829	1859	rBV	35120	78998	19.02%	2.392%
13	7.249	1917	1931	1963	rBV	160179	315145	75.87%	9.541%
14	7.561	2019	2028	2052	rBV2	19331	43514	10.48%	1.317%
15	7.876	2117	2126	2138	rBV4	2878	4892	1.18%	0.148%
16	8.031	2165	2174	2214	rBV	187813	415354	100.00%	12.575%
17	8.789	2399	2410	2429	rBV	193614	338462	81.49%	10.247%
18	10.159	2824	2836	2851	rBV	62536	102285	24.63%	3.097%
19	10.329	2881	2889	2897	rBV4	5048	7754	1.87%	0.235%
20	11.188	3145	3156	3176	rBV	197135	314441	75.70%	9.520%
21	11.564	3262	3273	3291	rVB	165057	264092	63.58%	7.995%




Sum of corrected areas: 3303010

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032386.D
Acq On : 11 Oct 2023 12:20
Operator : SY/MD
Sample : 04851-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

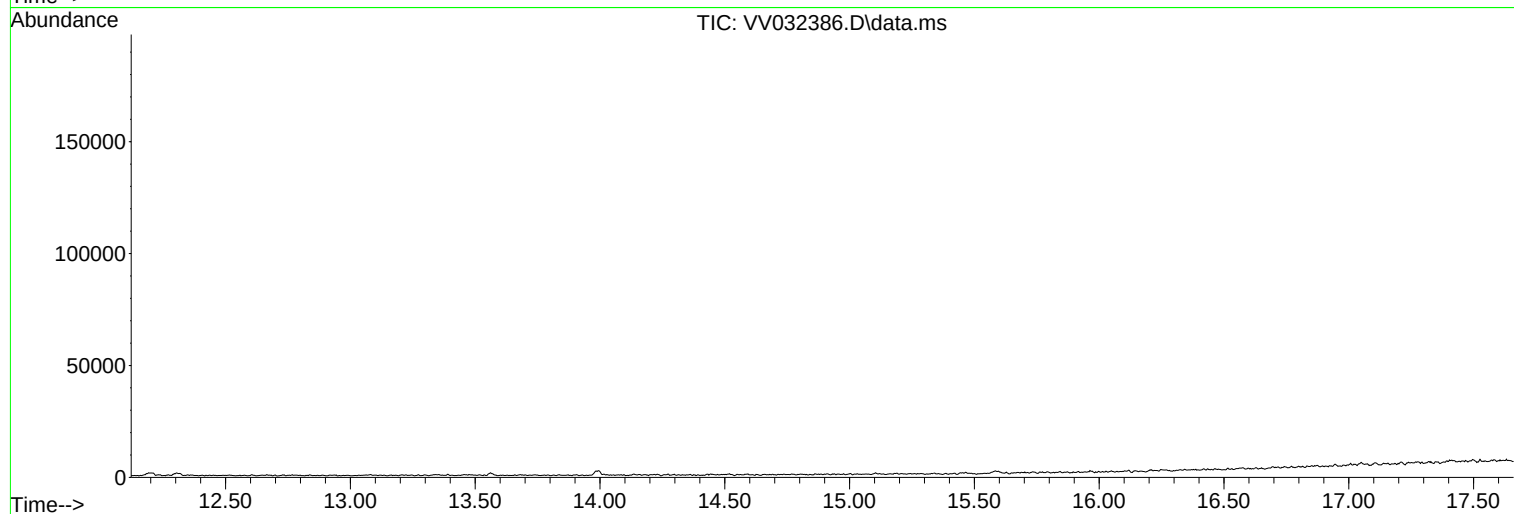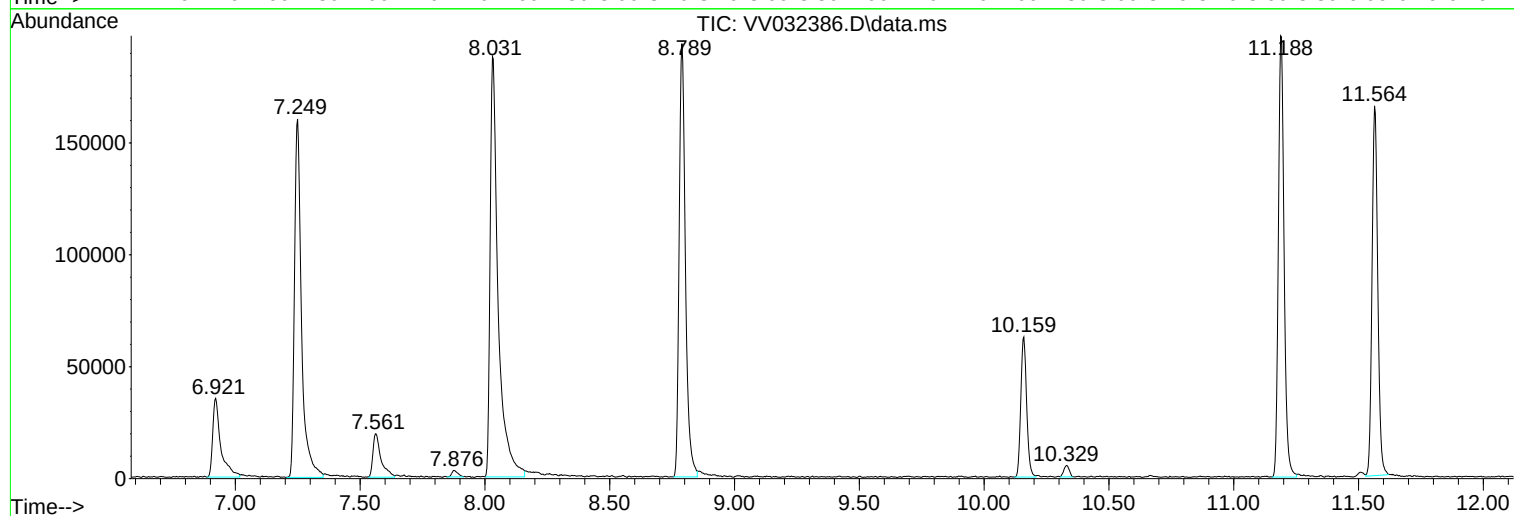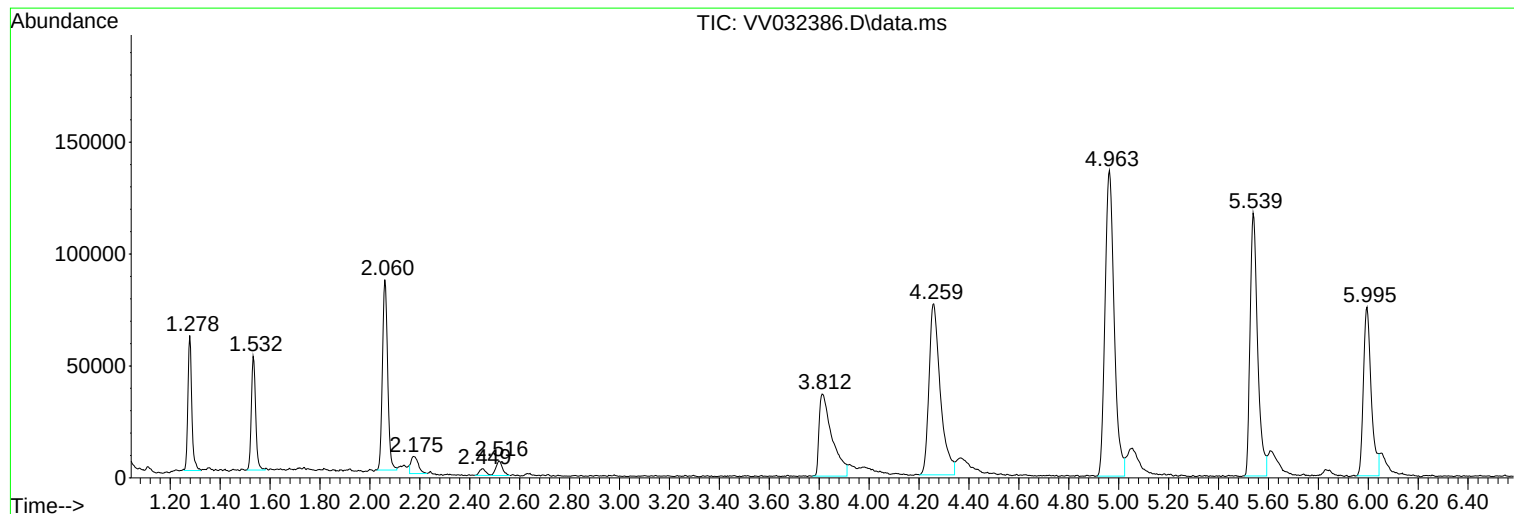

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032386.D
Acq On : 11 Oct 2023 12:20
Operator : SY/MD
Sample : 04851-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032386.D
Acq On : 11 Oct 2023 12:20
Operator : SY/MD
Sample : 04851-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc