

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
 Data File : VV032387.D
 Acq On : 11 Oct 2023 12:45
 Operator : SY/MD
 Sample : 04851-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B11

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032387.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	87	rVB	56016	58339	15.19%	1.845%
2	1.532	146	153	168	rVB	48438	57289	14.92%	1.811%
3	2.059	307	317	331	rBV	81734	118343	30.82%	3.742%
4	2.182	345	355	364	rVB3	6821	11439	2.98%	0.362%
5	2.452	427	439	448	rBV3	5367	9396	2.45%	0.297%
6	2.516	448	459	472	rVV3	10868	19475	5.07%	0.616%
7	3.809	852	861	895	rBV2	38269	130850	34.08%	4.137%
8	4.256	983	1000	1026	rBV2	58513	180174	46.92%	5.697%
9	4.963	1204	1220	1239	rBV2	128866	331327	86.29%	10.476%
10	5.538	1387	1399	1416	rBV	117425	246314	64.15%	7.788%
11	5.837	1483	1492	1494	rBV6	2897	4317	1.12%	0.136%
12	5.995	1527	1541	1554	rBV	74099	157464	41.01%	4.979%
13	6.921	1819	1829	1851	rBV2	32165	71637	18.66%	2.265%
14	7.249	1920	1931	1959	rBV	151671	294240	76.63%	9.304%
15	7.561	2018	2028	2051	rBV	19277	42446	11.05%	1.342%
16	7.879	2116	2127	2136	rBV3	3479	6247	1.63%	0.198%
17	8.030	2165	2174	2202	rBV	178560	383984	100.00%	12.141%
18	8.789	2398	2410	2432	rBV	197837	347254	90.43%	10.980%
19	10.159	2824	2836	2851	rBV	59472	97783	25.47%	3.092%
20	10.329	2881	2889	2899	rVB2	6513	9037	2.35%	0.286%
21	11.191	3146	3157	3183	rBV	206018	320187	83.39%	10.124%
22	11.503	3245	3254	3262	rBV7	3354	6754	1.76%	0.214%
23	11.564	3262	3273	3292	rVB	158922	258349	67.28%	8.169%




Sum of corrected areas: 3162645

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032387.D
Acq On : 11 Oct 2023 12:45
Operator : SY/MD
Sample : 04851-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

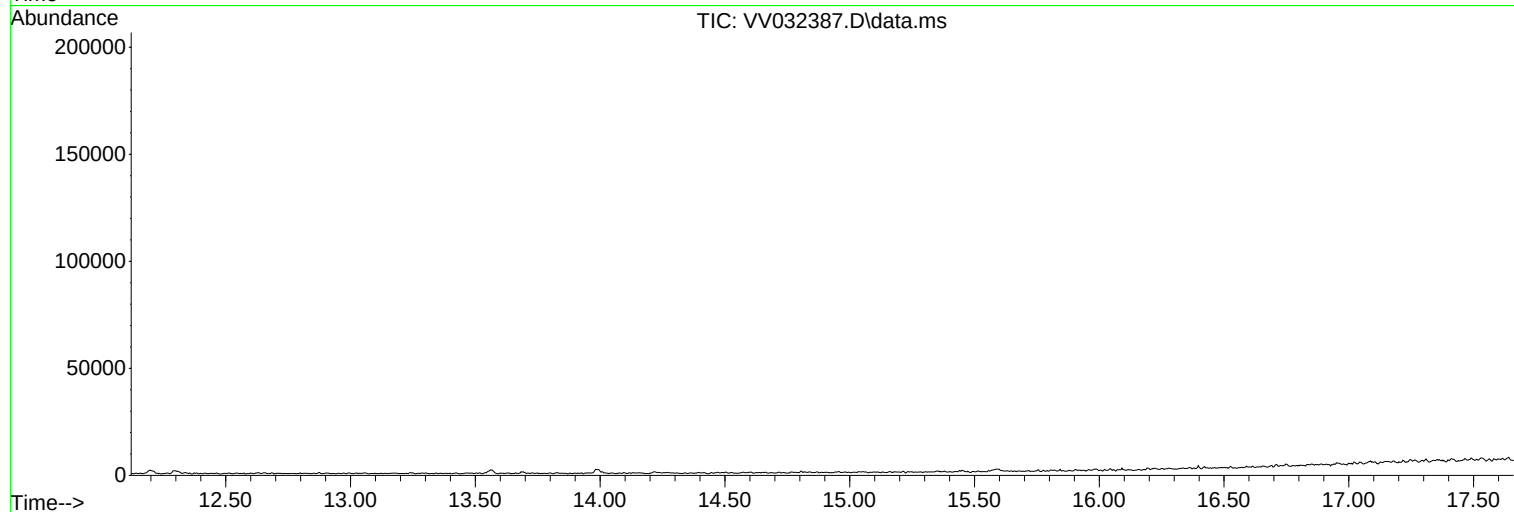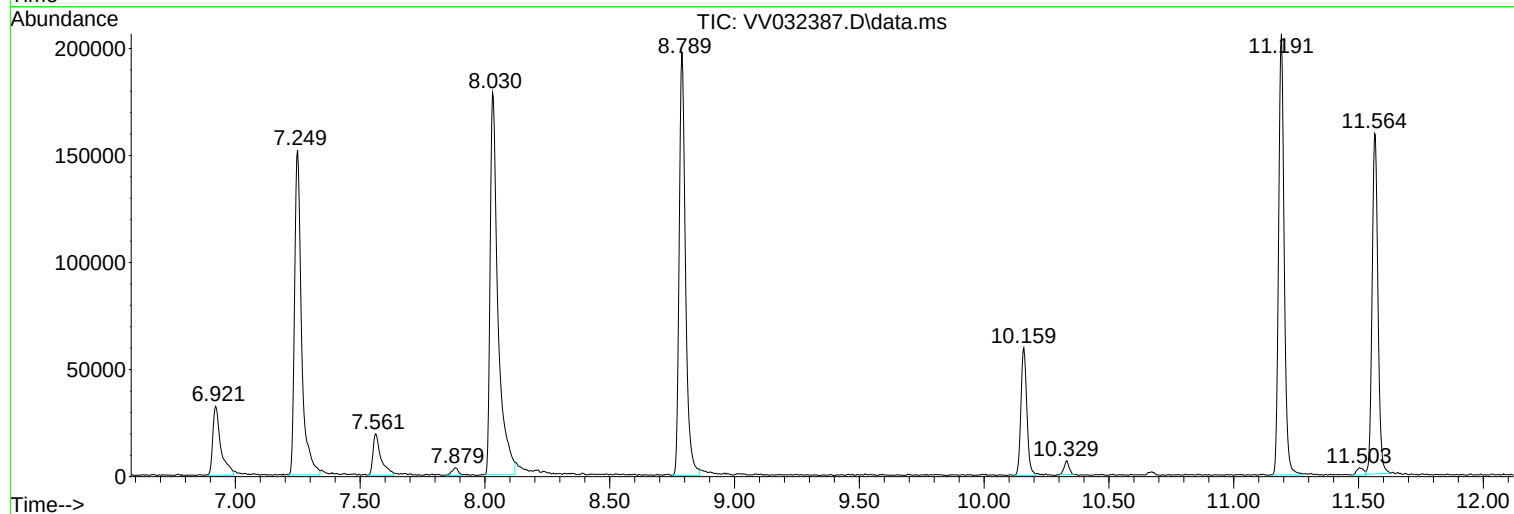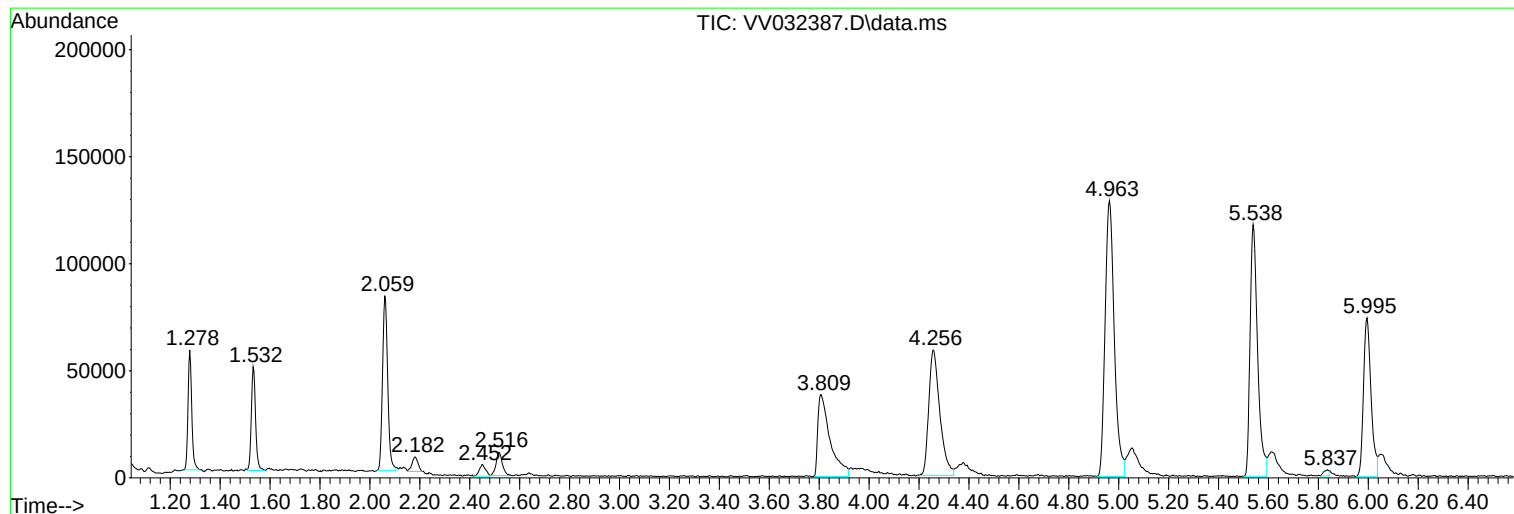

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032387.D
Acq On : 11 Oct 2023 12:45
Operator : SY/MD
Sample : 04851-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032387.D
Acq On : 11 Oct 2023 12:45
Operator : SY/MD
Sample : 04851-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc