

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
 Data File : VV032389.D
 Acq On : 11 Oct 2023 13:34
 Operator : SY/MD
 Sample : 04826-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCJV1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032389.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	86	rVB	58368	59600	15.10%	1.774%
2	1.532	145	153	163	rBV	45778	54735	13.87%	1.629%
3	2.060	307	317	332	rBV	81850	119798	30.35%	3.565%
4	2.175	347	353	363	rVB3	6397	11982	3.04%	0.357%
5	3.812	851	862	895	rBV	38053	139730	35.40%	4.158%
6	4.253	984	999	1024	rBV2	55707	153075	38.78%	4.555%
7	4.963	1203	1220	1238	rBV3	130373	331580	84.00%	9.867%
8	5.539	1388	1399	1415	rBV	126980	266215	67.44%	7.922%
9	5.838	1480	1492	1503	rBV8	3631	8976	2.27%	0.267%
10	5.992	1527	1540	1555	rBV	74000	160876	40.76%	4.787%
11	6.921	1819	1829	1853	rBV2	33498	73519	18.63%	2.188%
12	7.249	1918	1931	1963	rBV	151586	300324	76.09%	8.937%
13	7.561	2020	2028	2054	rBV	19319	40071	10.15%	1.192%
14	7.879	2117	2127	2145	rVB5	4806	12453	3.15%	0.371%
15	8.031	2165	2174	2209	rBV	179956	394716	100.00%	11.746%
16	8.789	2399	2410	2431	rBV	213702	372887	94.47%	11.097%
17	8.960	2454	2463	2472	rBV4	3844	6567	1.66%	0.195%
18	9.085	2492	2502	2512	rBV3	4867	9144	2.32%	0.272%
19	9.510	2619	2634	2651	rBV8	8227	22245	5.64%	0.662%
20	10.159	2824	2836	2849	rBV	59143	97497	24.70%	2.901%
21	10.329	2877	2889	2904	rBV2	11978	19248	4.88%	0.573%
22	11.104	3118	3130	3140	rBV9	2526	5458	1.38%	0.162%
23	11.188	3145	3156	3177	rBV	223024	361907	91.69%	10.770%
24	11.564	3262	3273	3300	rVB	165011	276021	69.93%	8.214%
25	12.198	3457	3470	3482	rBV2	7772	13730	3.48%	0.409%
26	12.291	3488	3499	3517	rBV2	14171	24437	6.19%	0.727%
27	13.204	3775	3783	3794	rBV2	10603	15899	4.03%	0.473%
28	13.989	4019	4027	4039	rVB2	4462	7693	1.95%	0.229%




Sum of corrected areas: 3360383

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032389.D
Acq On : 11 Oct 2023 13:34
Operator : SY/MD
Sample : 04826-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJV1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

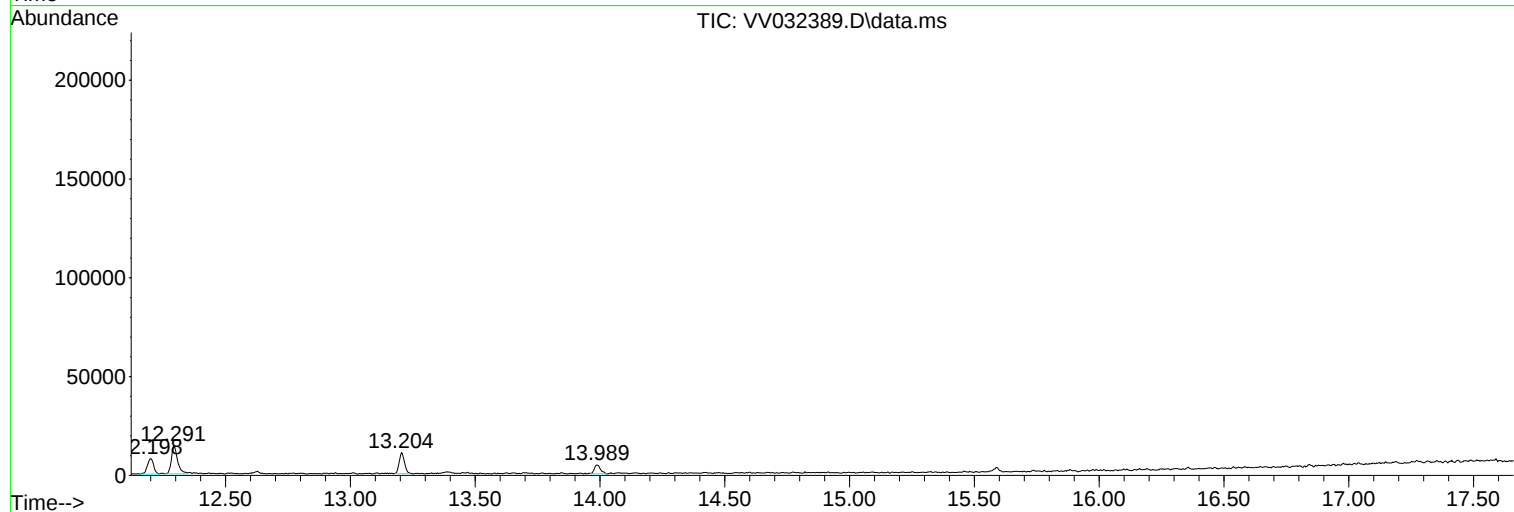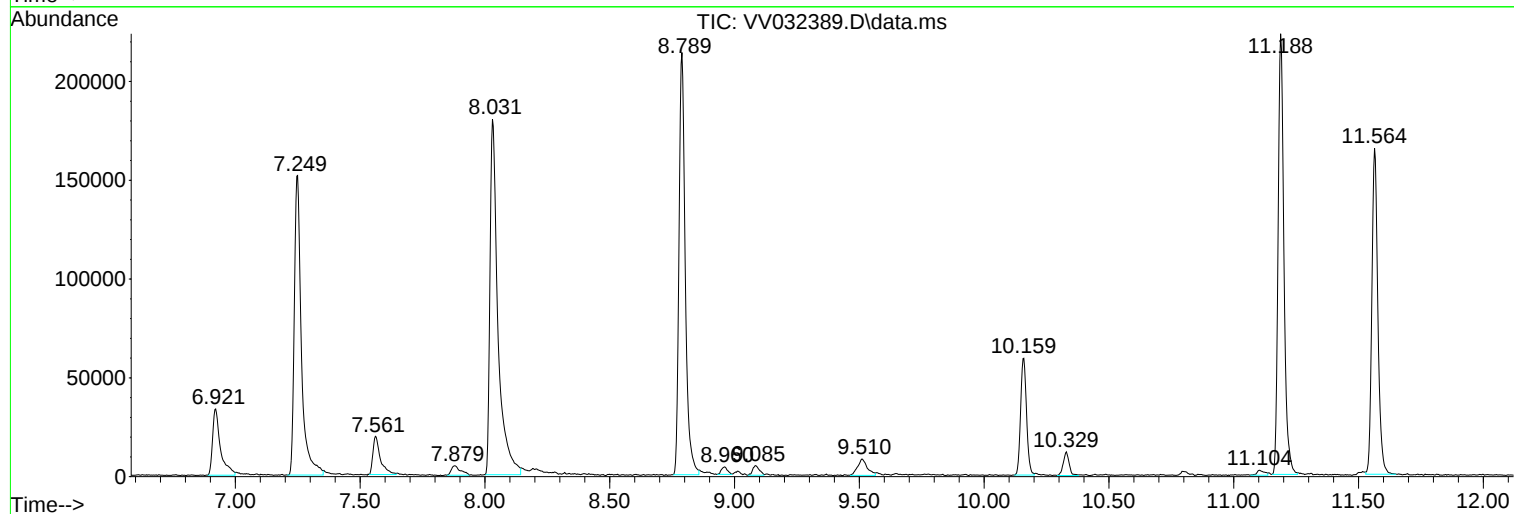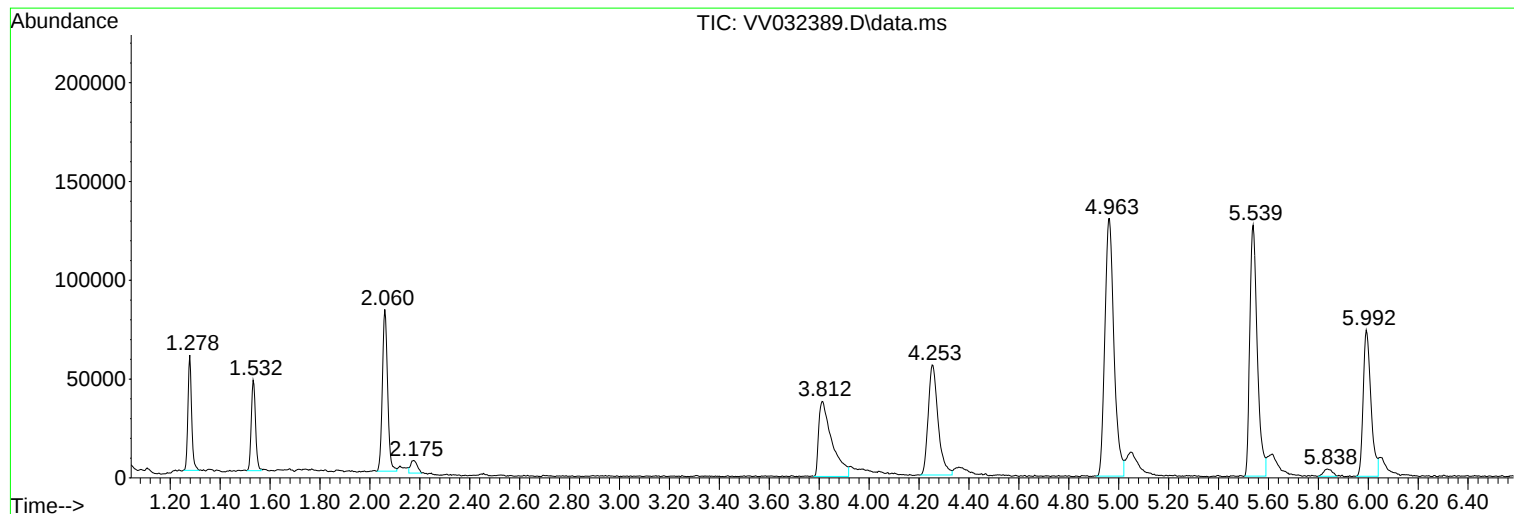

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032389.D
Acq On : 11 Oct 2023 13:34
Operator : SY/MD
Sample : 04826-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJV1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032389.D
Acq On : 11 Oct 2023 13:34
Operator : SY/MD
Sample : 04826-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJV1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------