

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
 Data File : VV032390.D
 Acq On : 11 Oct 2023 13:58
 Operator : SY/MD
 Sample : 04826-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCJV2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032390.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	84	rBV	60258	63022	14.72%	1.816%
2	1.532	145	153	166	rBV	51047	60328	14.09%	1.739%
3	2.060	306	317	332	rBV	85622	127276	29.72%	3.668%
4	2.175	347	353	370	rVB3	6449	12990	3.03%	0.374%
5	3.806	850	860	897	rBV	43478	151221	35.31%	4.358%
6	4.253	983	999	1021	rBV	59189	161183	37.64%	4.645%
7	4.960	1201	1219	1239	rBV2	134700	351395	82.05%	10.127%
8	5.539	1387	1399	1415	rBV	127577	265624	62.02%	7.655%
9	5.992	1528	1540	1555	rBV2	76773	170871	39.90%	4.924%
10	6.918	1818	1828	1849	rBV2	35573	77156	18.02%	2.224%
11	7.246	1919	1930	1953	rBV	159900	309207	72.20%	8.911%
12	7.558	2017	2027	2046	rBV3	19796	43711	10.21%	1.260%
13	7.879	2115	2127	2143	rBV3	16844	31096	7.26%	0.896%
14	8.031	2165	2174	2219	rBV	195555	428259	100.00%	12.342%
15	8.789	2398	2410	2436	rBV	208887	371131	86.66%	10.696%
16	9.011	2469	2479	2487	rBV4	3208	5228	1.22%	0.151%
17	9.513	2621	2635	2649	rBV7	5058	12352	2.88%	0.356%
18	10.156	2823	2835	2853	rBV	63399	105040	24.53%	3.027%
19	10.326	2878	2888	2902	rVB	28028	45592	10.65%	1.314%
20	11.188	3144	3156	3177	rBV	215899	350358	81.81%	10.097%
21	11.564	3262	3273	3294	rVB	174079	281708	65.78%	8.119%
22	12.198	3458	3470	3483	rVB	14575	23209	5.42%	0.669%
23	12.294	3489	3500	3511	rBV7	7519	13687	3.20%	0.394%
24	13.992	4017	4028	4035	rBV	4912	8218	1.92%	0.237%




Sum of corrected areas: 3469862

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032390.D
Acq On : 11 Oct 2023 13:58
Operator : SY/MD
Sample : 04826-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJV2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

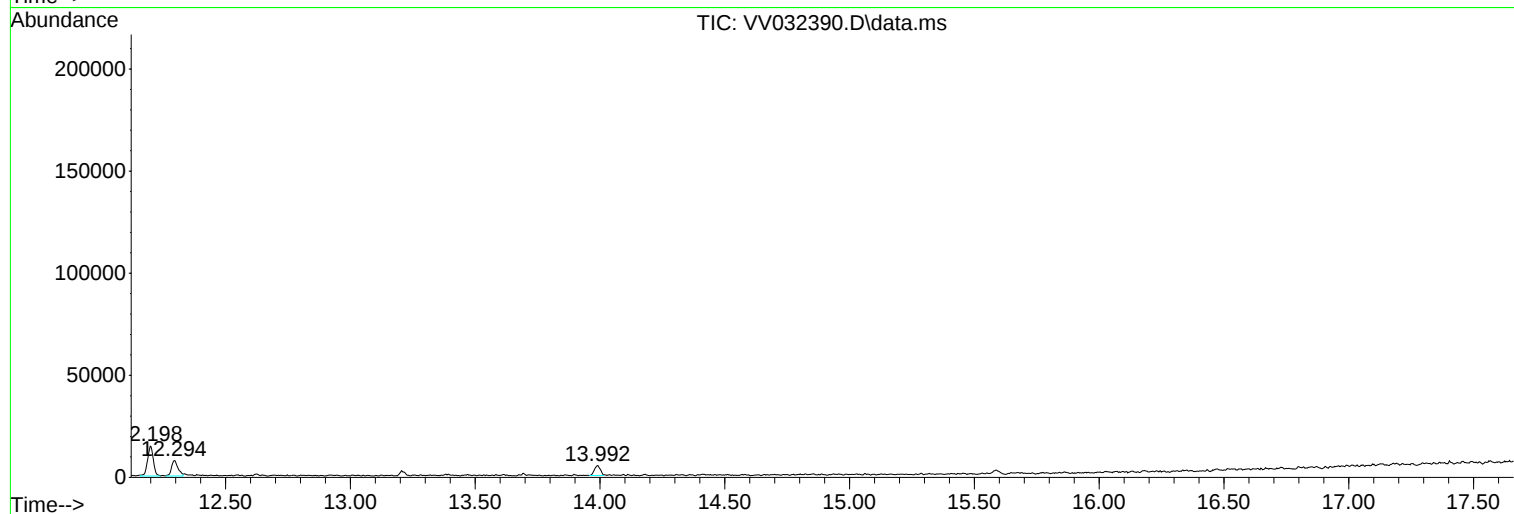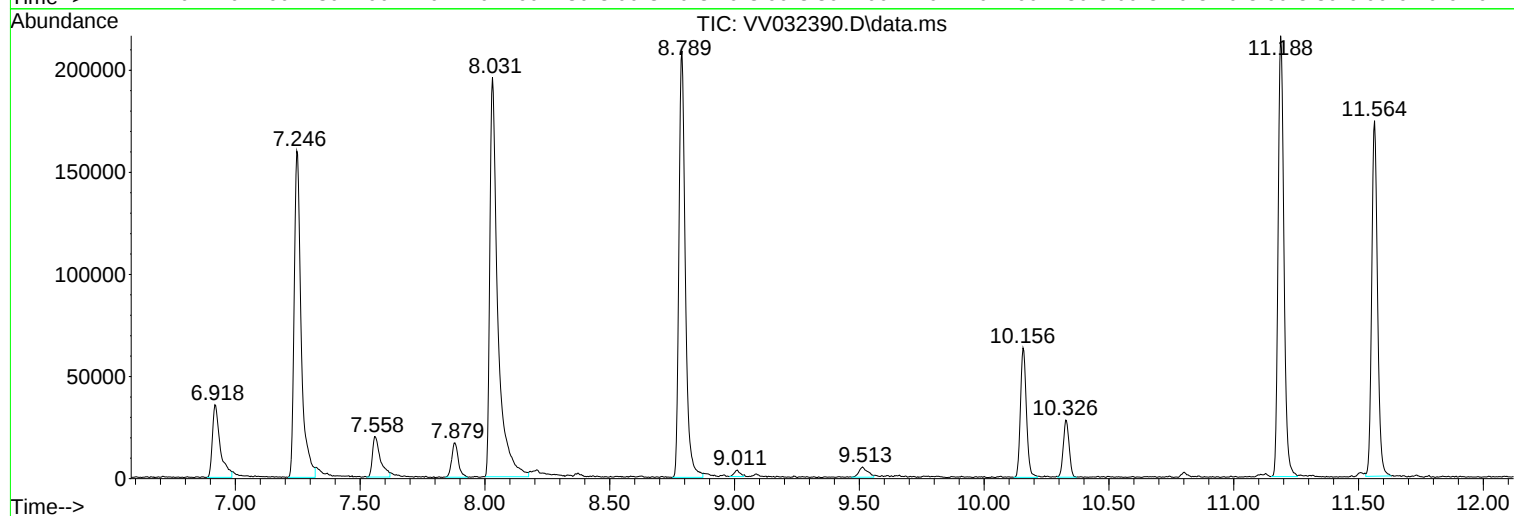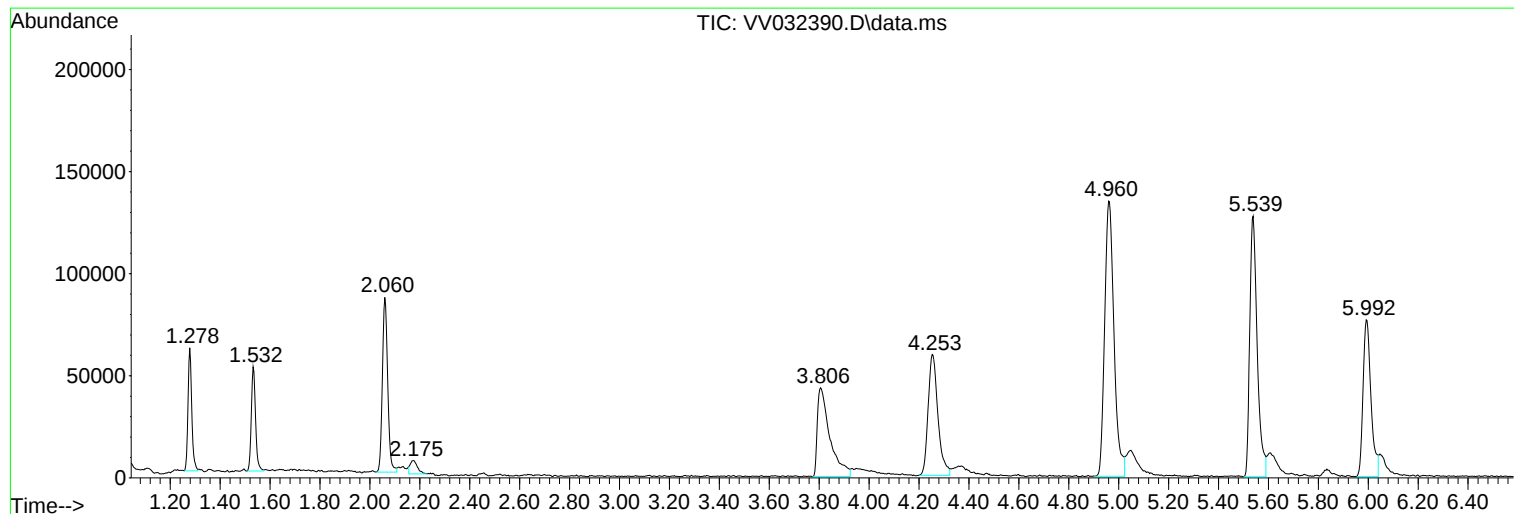

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032390.D
Acq On : 11 Oct 2023 13:58
Operator : SY/MD
Sample : 04826-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJV2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032390.D
Acq On : 11 Oct 2023 13:58
Operator : SY/MD
Sample : 04826-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJV2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc