

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
 Data File : VV032393.D
 Acq On : 11 Oct 2023 15:11
 Operator : SY/MD
 Sample : 04851-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B03

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032393.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	16	21	30	rVB	5155	6947	1.61%	0.203%
2	1.278	66	74	90	rBV	59245	64445	14.95%	1.886%
3	1.532	145	153	168	rBV	51264	61203	14.20%	1.791%
4	2.060	306	317	331	rBV	87902	129966	30.15%	3.804%
5	2.172	346	352	368	rVB2	6617	14267	3.31%	0.418%
6	3.809	851	861	899	rBV2	42501	152314	35.34%	4.458%
7	4.256	983	1000	1020	rBV	60364	167978	38.97%	4.916%
8	4.362	1027	1033	1045	rVB5	2676	5024	1.17%	0.147%
9	4.960	1205	1219	1238	rBV2	135896	352046	81.67%	10.304%
10	5.539	1387	1399	1415	rBV	116693	246009	57.07%	7.200%
11	5.841	1480	1493	1501	rBV7	2447	5092	1.18%	0.149%
12	5.992	1523	1540	1554	rBV	78493	167906	38.95%	4.914%
13	6.442	1669	1680	1694	rBV3	10764	22701	5.27%	0.664%
14	6.921	1819	1829	1856	rBV2	34555	78788	18.28%	2.306%
15	7.246	1918	1930	1951	rBV	160795	308592	71.59%	9.032%
16	7.561	2019	2028	2049	rBV2	20653	43532	10.10%	1.274%
17	7.879	2117	2127	2128	rBV2	5953	6278	1.46%	0.184%
18	7.908	2128	2136	2154	rVB3	22336	45295	10.51%	1.326%
19	8.030	2163	2174	2212	rBV	201281	431052	100.00%	12.616%
20	8.182	2212	2221	2234	rVB2	15068	30284	7.03%	0.886%
21	8.789	2395	2410	2436	rBV	200260	345945	80.26%	10.125%
22	9.677	2677	2686	2697	rVB2	3867	6596	1.53%	0.193%
23	10.156	2825	2835	2851	rBV	65088	107711	24.99%	3.152%
24	10.329	2878	2889	2898	rBV2	10261	15475	3.59%	0.453%
25	11.188	3145	3156	3182	rBV	203049	322026	74.71%	9.425%
26	11.564	3261	3273	3291	rBV	170014	271470	62.98%	7.945%
27	12.197	3460	3470	3480	rVB	4899	7747	1.80%	0.227%




Sum of corrected areas: 3416689

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032393.D
Acq On : 11 Oct 2023 15:11
Operator : SY/MD
Sample : 04851-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

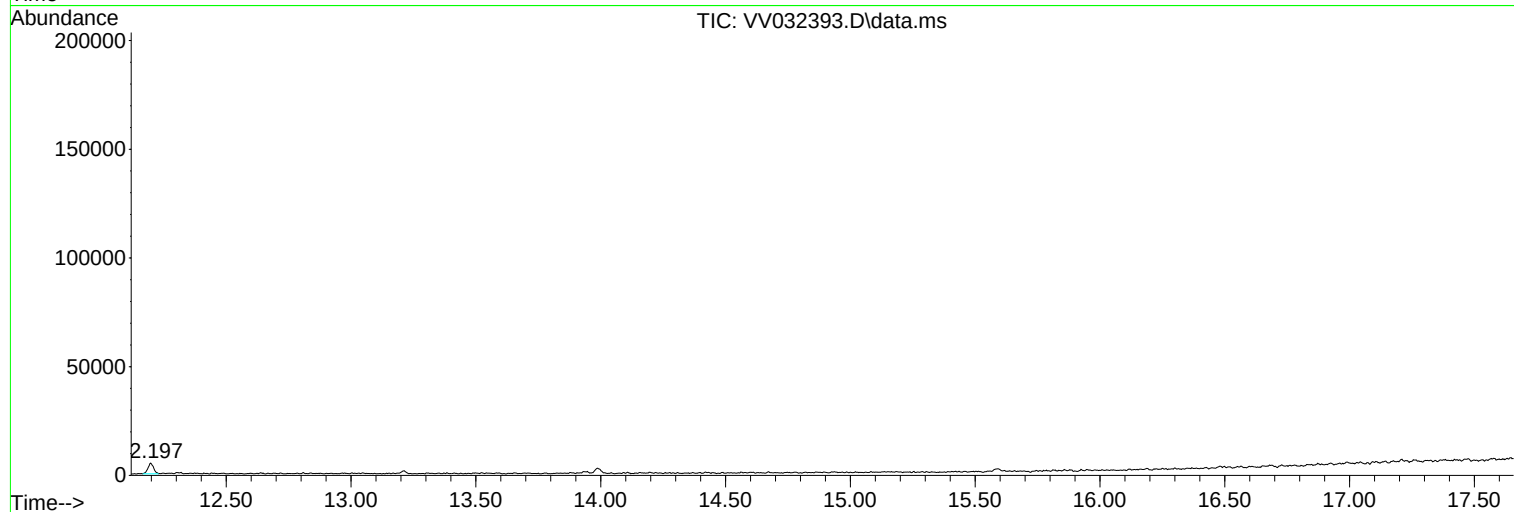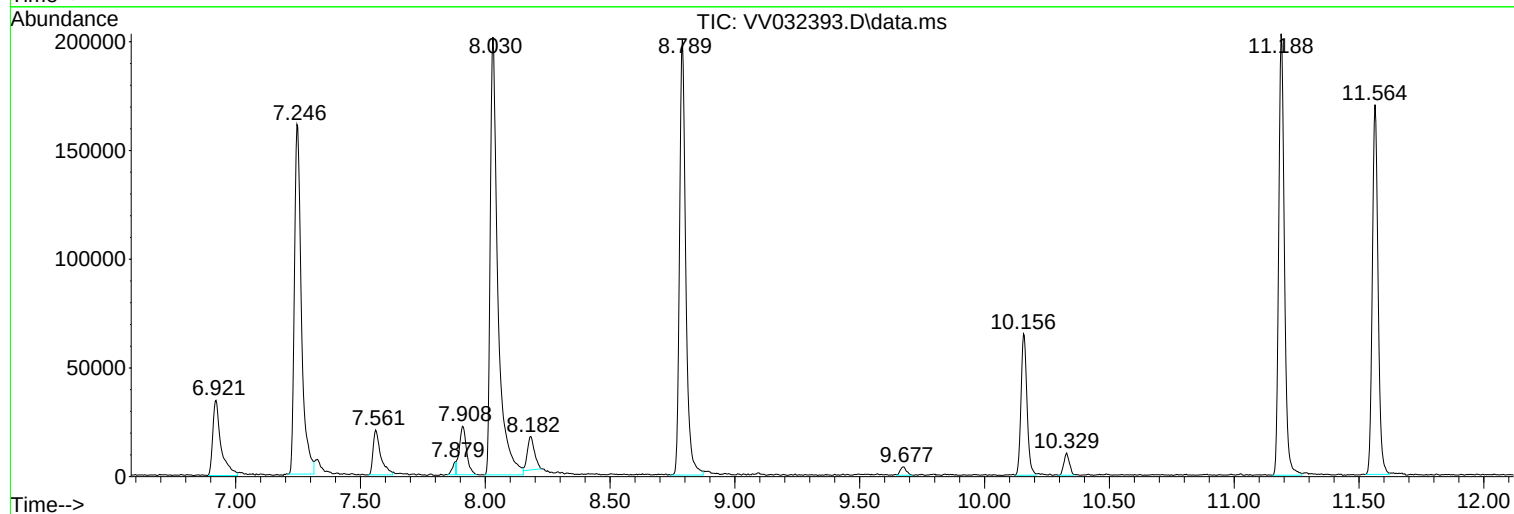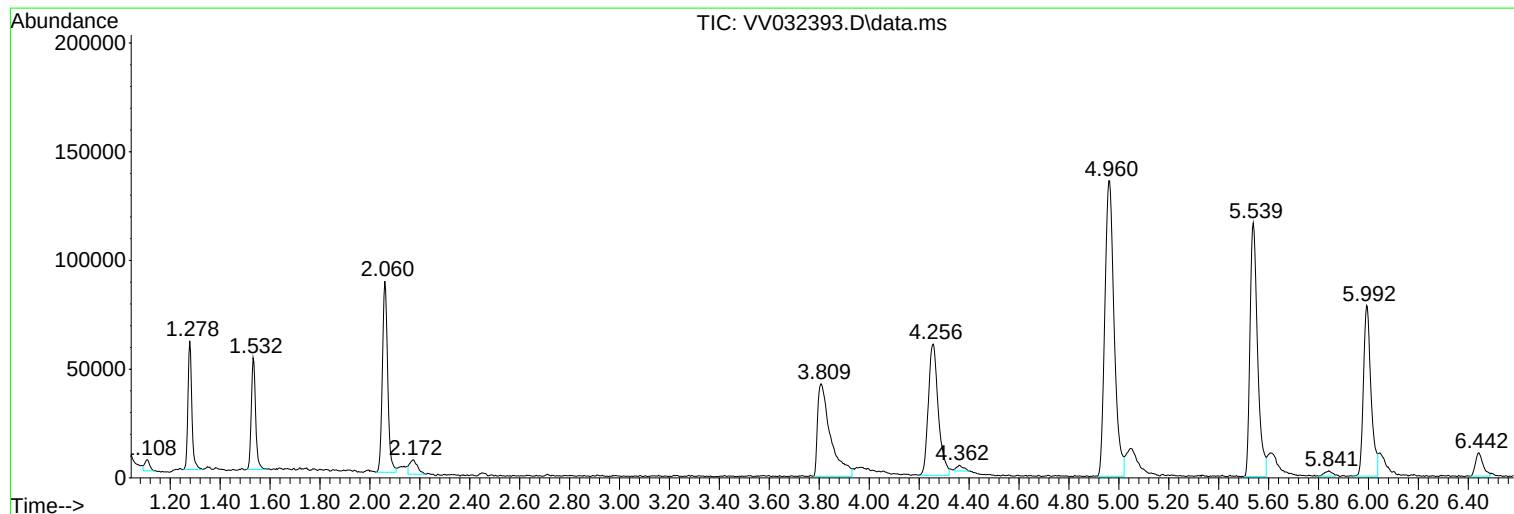

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032393.D
Acq On : 11 Oct 2023 15:11
Operator : SY/MD
Sample : 04851-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032393.D
Acq On : 11 Oct 2023 15:11
Operator : SY/MD
Sample : 04851-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
