

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
 Data File : VV032394.D
 Acq On : 11 Oct 2023 15:33
 Operator : SY/MD
 Sample : 04851-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B04

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	30	rVB	5068	7060	1.74%	0.193%
2	1.278	66	74	87	rBV	55392	59840	14.77%	1.638%
3	1.352	91	97	105	rBV4	2945	4062	1.00%	0.111%
4	1.532	146	153	164	rVB	48058	54309	13.41%	1.487%
5	2.060	307	317	332	rBV	83252	121571	30.01%	3.328%
6	2.172	345	352	370	rVB5	5953	12494	3.08%	0.342%
7	3.809	848	861	890	rBV	40140	133289	32.90%	3.649%
8	4.259	985	1001	1027	rBV3	63917	213244	52.64%	5.838%
9	4.963	1205	1220	1238	rBV2	129068	331005	81.71%	9.062%
10	5.539	1388	1399	1417	rBV	131202	276634	68.29%	7.574%
11	5.834	1480	1491	1504	rVB10	2699	6169	1.52%	0.169%
12	5.992	1524	1540	1554	rBV2	74989	161602	39.89%	4.424%
13	6.439	1667	1679	1692	rBV2	48838	98252	24.25%	2.690%
14	6.921	1816	1829	1858	rBV	33573	74267	18.33%	2.033%
15	7.249	1919	1931	1953	rBV	152314	296205	73.12%	8.110%
16	7.561	2020	2028	2047	rBV	20121	41031	10.13%	1.123%
17	7.908	2117	2136	2162	rBV3	54558	111889	27.62%	3.063%
18	8.030	2165	2174	2210	rBV	190872	405110	100.00%	11.091%
19	8.182	2210	2221	2241	rVB2	45845	91168	22.50%	2.496%
20	8.789	2399	2410	2432	rBV	217755	381101	94.07%	10.434%
21	9.670	2675	2684	2699	rBV2	10388	18137	4.48%	0.497%
22	10.159	2825	2836	2848	rBV2	63669	102850	25.39%	2.816%
23	10.329	2879	2889	2899	rVB2	9733	14852	3.67%	0.407%
24	11.188	3145	3156	3177	rBV	219601	357874	88.34%	9.798%
25	11.564	3262	3273	3298	rVB	162631	264795	65.36%	7.250%
26	12.201	3459	3471	3480	rVB2	4420	8106	2.00%	0.222%
27	13.988	4020	4027	4036	rVB2	3451	5573	1.38%	0.153%




Sum of corrected areas: 3652489

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032394.D
Acq On : 11 Oct 2023 15:33
Operator : SY/MD
Sample : 04851-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

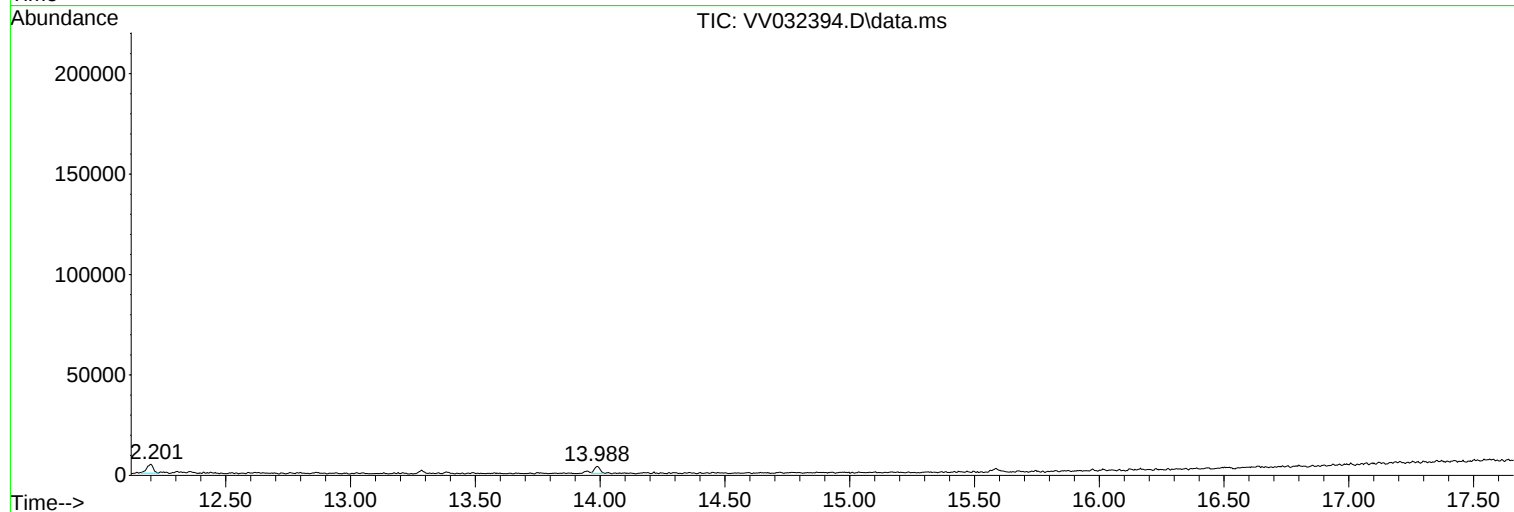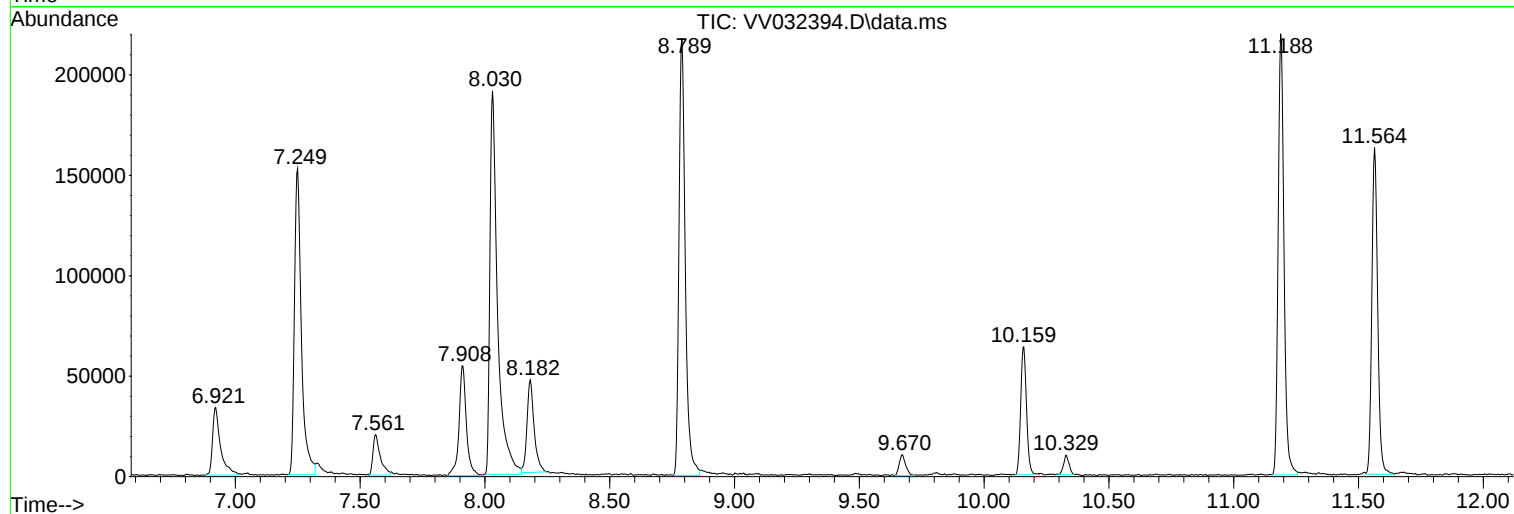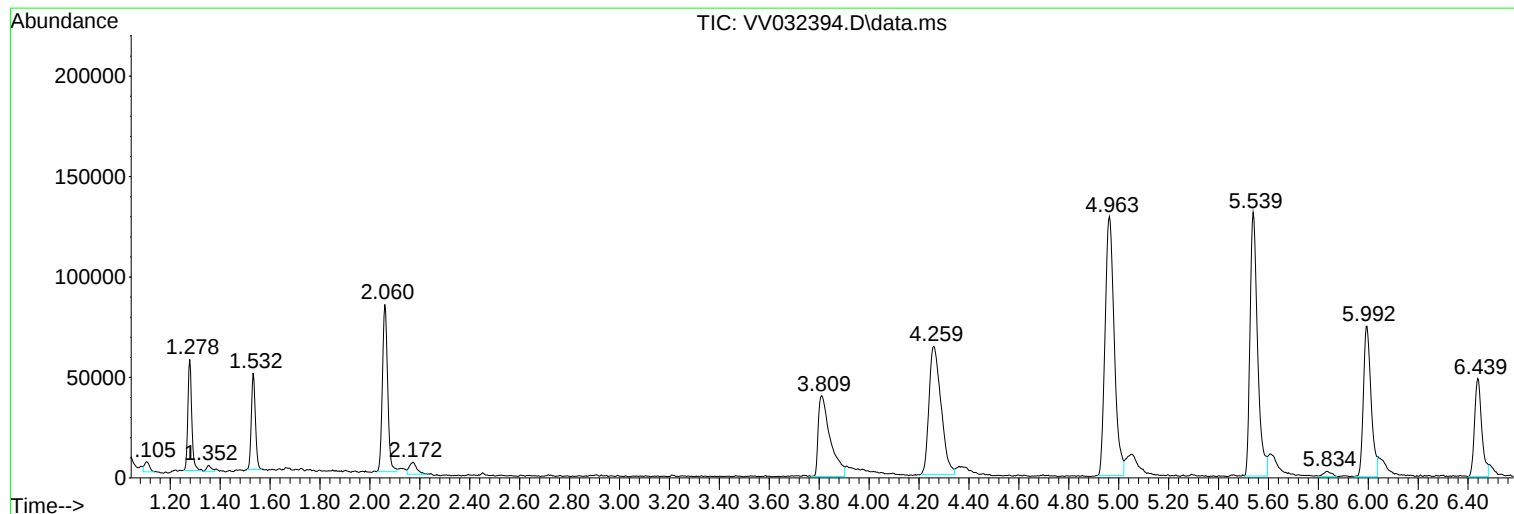

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032394.D
Acq On : 11 Oct 2023 15:33
Operator : SY/MD
Sample : 04851-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032394.D
Acq On : 11 Oct 2023 15:33
Operator : SY/MD
Sample : 04851-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------