

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV101123\  
 Data File : VV032395.D  
 Acq On : 11 Oct 2023 15:57  
 Operator : SY/MD  
 Sample : 04851-04  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0B05

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032395.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.278       | 67            | 74          | 89           | rVB      | 54917          | 58591         | 3.87%           | 1.273%        |
| 2         | 1.532       | 146           | 153         | 167          | rVB      | 48647          | 56415         | 3.72%           | 1.226%        |
| 3         | 2.060       | 308           | 317         | 331          | rBV      | 80323          | 117760        | 7.77%           | 2.559%        |
| 4         | 3.809       | 852           | 861         | 893          | rBV2     | 40700          | 135123        | 8.91%           | 2.936%        |
| 5         | 4.256       | 984           | 1000        | 1025         | rBV2     | 55606          | 151558        | 10.00%          | 3.293%        |
| 6         | 4.963       | 1203          | 1220        | 1238         | rBV2     | 127302         | 329055        | 21.71%          | 7.150%        |
| 7         | 5.539       | 1386          | 1399        | 1415         | rBV      | 112495         | 236767        | 15.62%          | 5.145%        |
| 8         | 5.992       | 1526          | 1540        | 1556         | rBV2     | 74592          | 162607        | 10.73%          | 3.533%        |
| 9         | 6.921       | 1819          | 1829        | 1858         | rBV      | 31854          | 73774         | 4.87%           | 1.603%        |
| 10        | 7.246       | 1916          | 1930        | 1950         | rBV      | 150175         | 288052        | 19.00%          | 6.259%        |
| 11        | 7.561       | 2013          | 2028        | 2046         | rBV      | 19042          | 41888         | 2.76%           | 0.910%        |
| 12        | 7.908       | 2116          | 2136        | 2163         | rBV      | 828267         | 1515704       | 100.00%         | 32.936%       |
| 13        | 8.031       | 2164          | 2174        | 2209         | rVV      | 196422         | 406592        | 26.83%          | 8.835%        |
| 14        | 8.789       | 2399          | 2410        | 2435         | rBV      | 193743         | 337871        | 22.29%          | 7.342%        |
| 15        | 10.156      | 2825          | 2835        | 2850         | rBV2     | 62090          | 101557        | 6.70%           | 2.207%        |
| 16        | 10.329      | 2877          | 2889        | 2900         | rBV3     | 10718          | 16943         | 1.12%           | 0.368%        |
| 17        | 11.188      | 3145          | 3156        | 3176         | rBV      | 200202         | 315068        | 20.79%          | 6.846%        |
| 18        | 11.564      | 3262          | 3273        | 3289         | rBV      | 160827         | 256585        | 16.93%          | 5.576%        |




Sum of corrected areas: 4601910

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV101123\  
Data File : VV032395.D  
Acq On : 11 Oct 2023 15:57  
Operator : SY/MD  
Sample : 04851-04  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0B05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092923WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

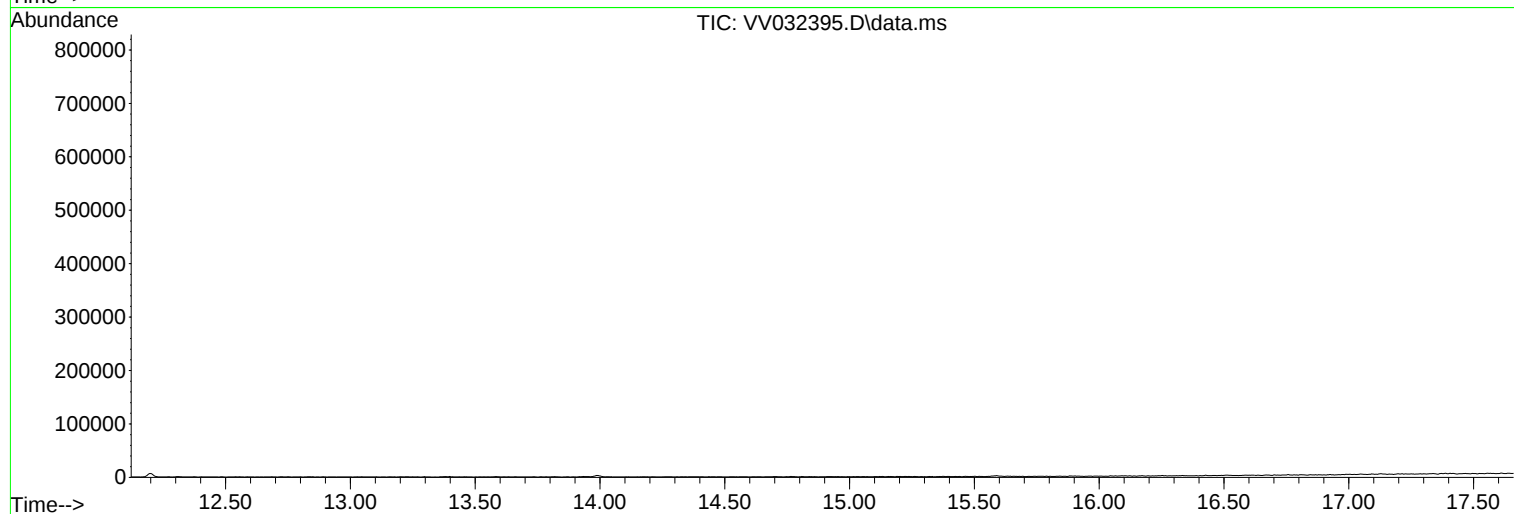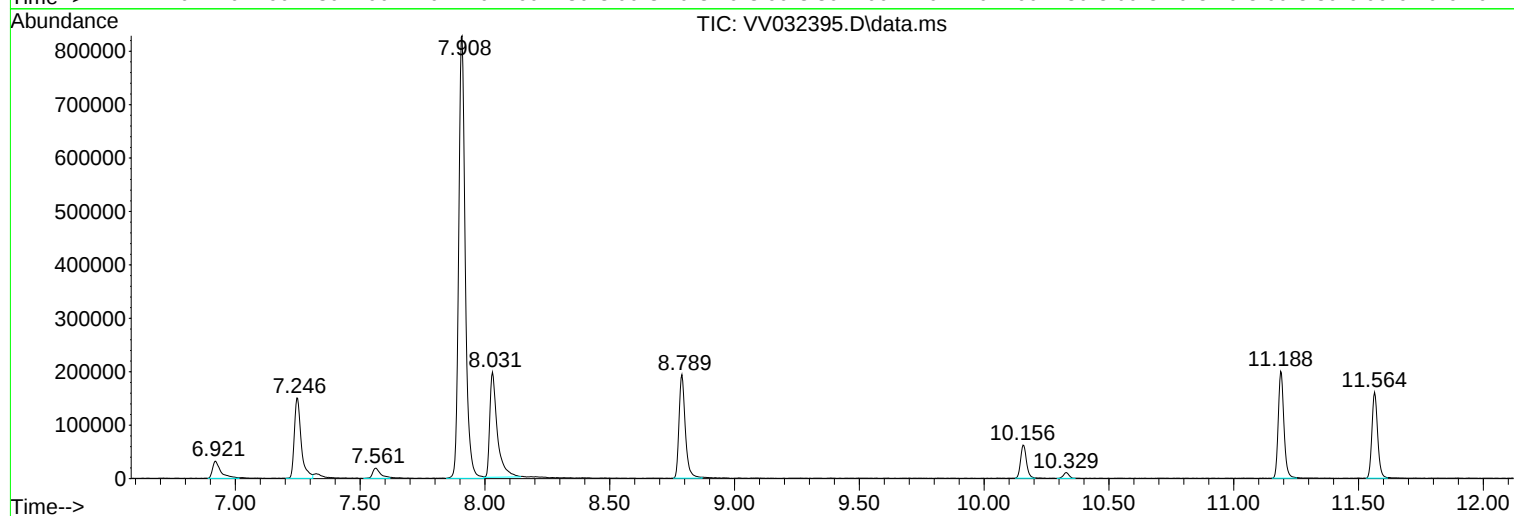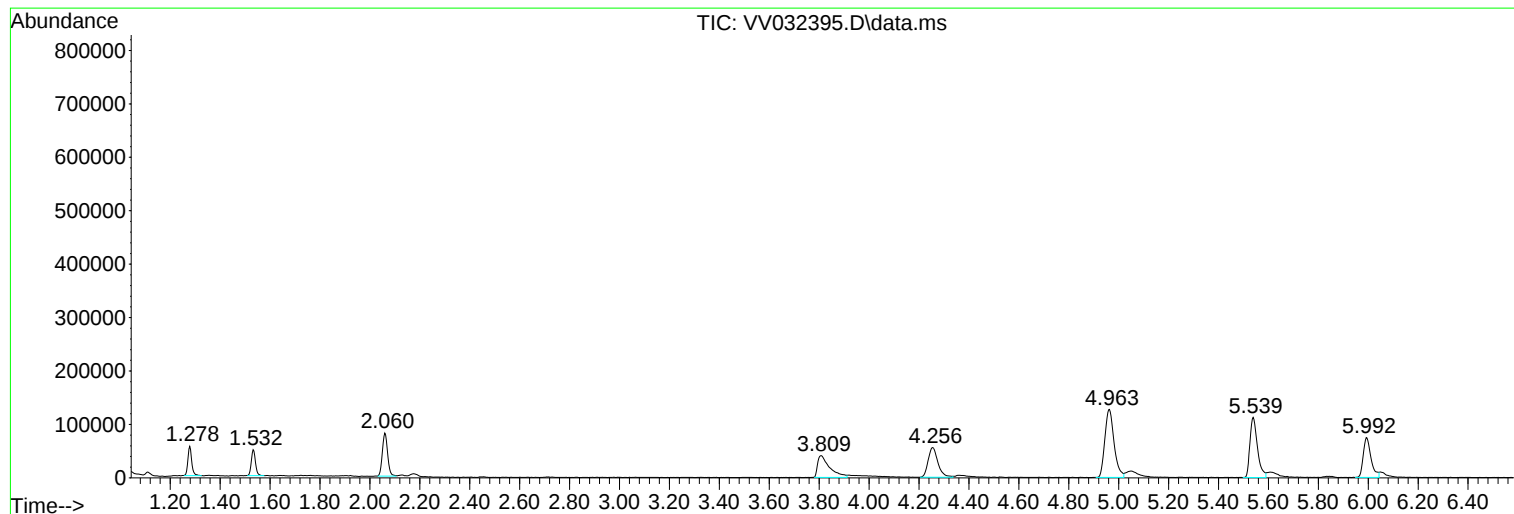

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV101123\  
Data File : VV032395.D  
Acq On : 11 Oct 2023 15:57  
Operator : SY/MD  
Sample : 04851-04  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0B05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092923WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV101123\  
Data File : VV032395.D  
Acq On : 11 Oct 2023 15:57  
Operator : SY/MD  
Sample : 04851-04  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0B05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092923WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |