

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
 Data File : VV032398.D
 Acq On : 11 Oct 2023 17:07
 Operator : SY/MD
 Sample : 04851-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B08

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032398.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	30	rVB	5053	7077	1.72%	0.206%
2	1.278	67	74	88	rVB	53924	57757	14.01%	1.681%
3	1.532	146	153	166	rVB	46173	55101	13.36%	1.604%
4	2.060	307	317	332	rBV	78407	116659	28.29%	3.395%
5	2.182	347	355	365	rVB3	6505	12976	3.15%	0.378%
6	3.809	852	861	892	rBV2	38149	134724	32.67%	3.921%
7	4.259	984	1001	1024	rBV4	64481	209000	50.68%	6.083%
8	4.963	1205	1220	1240	rBV3	128379	329420	79.89%	9.587%
9	5.539	1387	1399	1415	rBV	114603	235691	57.16%	6.859%
10	5.838	1482	1492	1501	rBV7	2118	4640	1.13%	0.135%
11	5.992	1528	1540	1554	rBV	72843	155866	37.80%	4.536%
12	6.439	1666	1679	1704	rBV	43068	94875	23.01%	2.761%
13	6.921	1819	1829	1859	rBV2	33120	72948	17.69%	2.123%
14	7.246	1918	1930	1953	rBV	145375	283501	68.75%	8.251%
15	7.561	2019	2028	2045	rBV2	19279	40147	9.74%	1.168%
16	7.908	2117	2136	2154	rBV3	42241	90584	21.97%	2.636%
17	8.030	2163	2174	2211	rBV	192061	412365	100.00%	12.001%
18	8.181	2211	2221	2237	rVB	39283	79210	19.21%	2.305%
19	8.789	2399	2410	2435	rBV	190364	335239	81.30%	9.757%
20	9.670	2675	2684	2699	rVB3	8902	16139	3.91%	0.470%
21	10.156	2824	2835	2853	rBV	62728	102626	24.89%	2.987%
22	10.329	2879	2889	2902	rBV3	12860	20197	4.90%	0.588%
23	11.188	3146	3156	3180	rBV	192928	311062	75.43%	9.053%
24	11.564	3260	3273	3291	rBV	156881	248119	60.17%	7.221%
25	12.194	3461	3469	3477	rVB2	3579	5454	1.32%	0.159%
26	13.992	4019	4028	4037	rBV	2738	4623	1.12%	0.135%




Sum of corrected areas: 3436000

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032398.D
Acq On : 11 Oct 2023 17:07
Operator : SY/MD
Sample : 04851-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

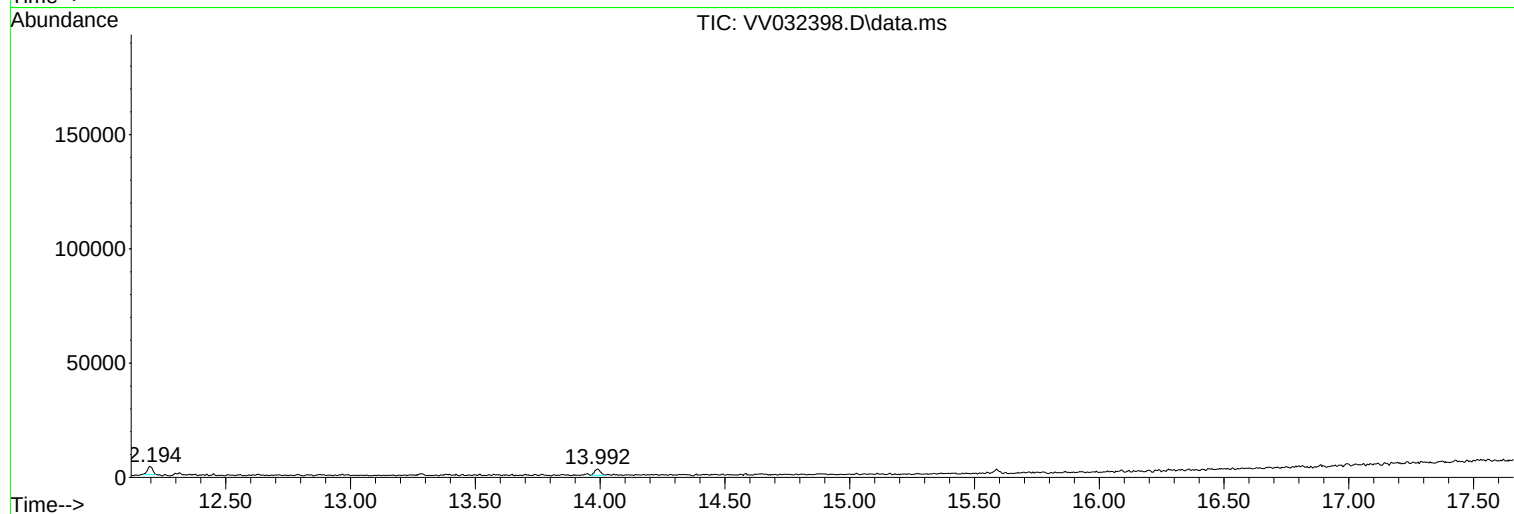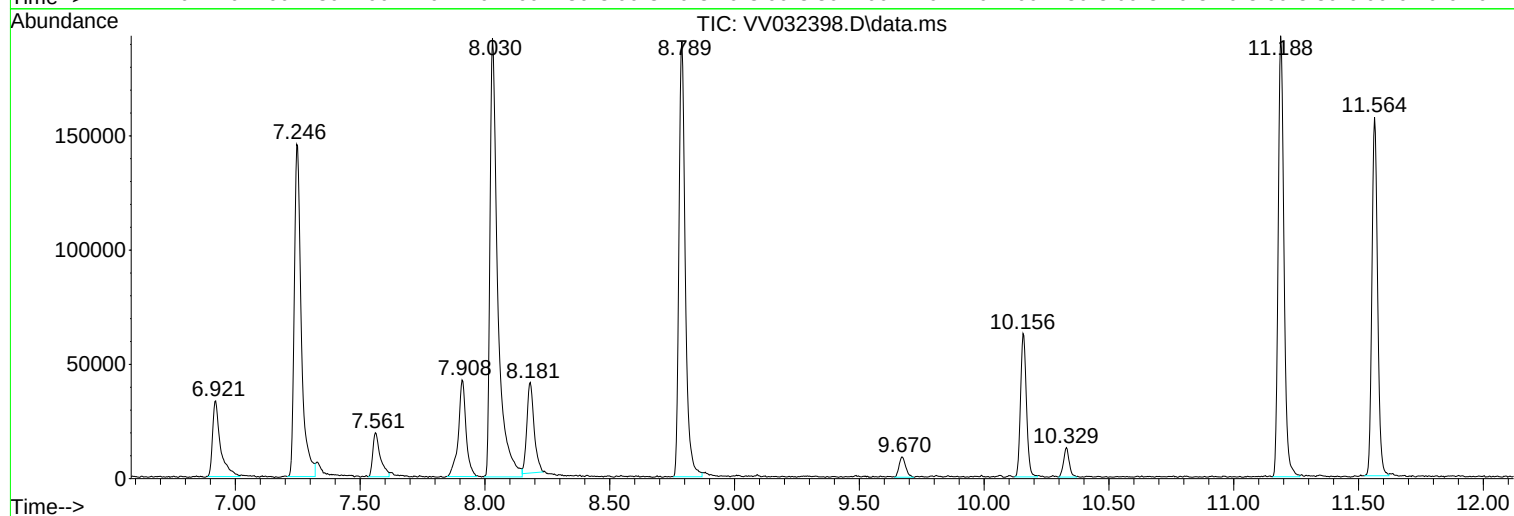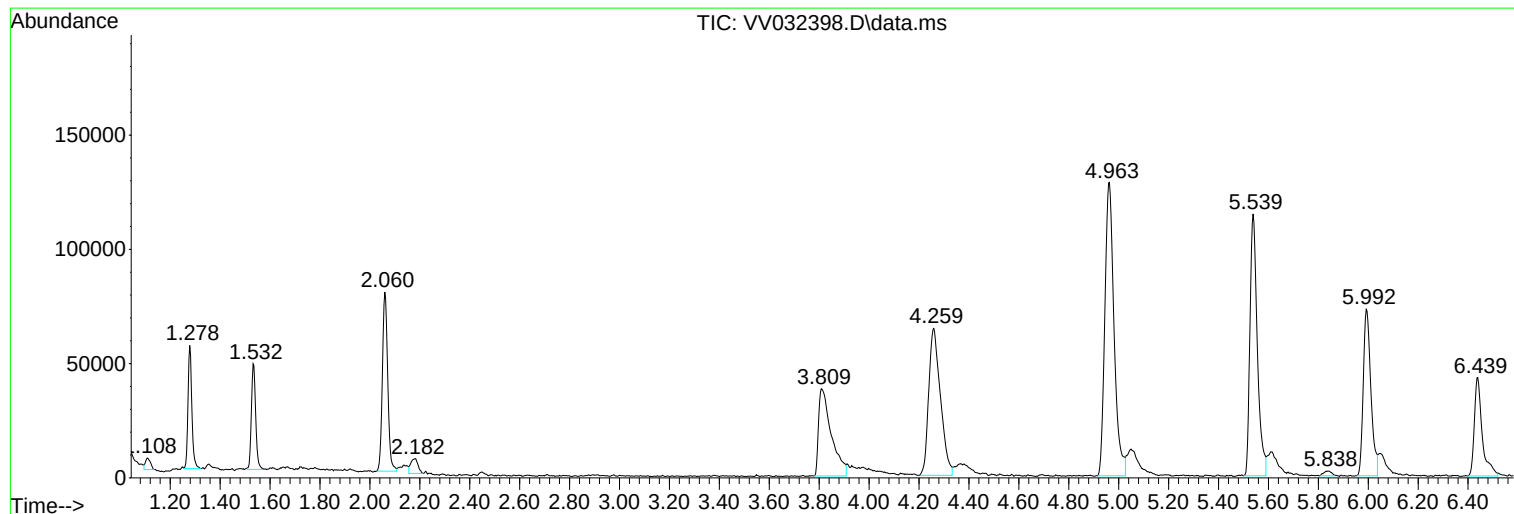

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032398.D
Acq On : 11 Oct 2023 17:07
Operator : SY/MD
Sample : 04851-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032398.D
Acq On : 11 Oct 2023 17:07
Operator : SY/MD
Sample : 04851-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B08

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc