

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
 Data File : VV032399.D
 Acq On : 11 Oct 2023 17:31
 Operator : SY/MD
 Sample : 04851-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B09

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032399.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	16	22	31	rVB	5002	7076	1.72%	0.222%
2	1.278	67	74	87	rVB	54461	57909	14.05%	1.814%
3	1.532	144	153	161	rBV	48695	56744	13.77%	1.777%
4	2.060	307	317	333	rBV	80506	119076	28.89%	3.729%
5	2.175	347	353	366	rVB3	5522	10685	2.59%	0.335%
6	3.812	848	862	897	rBV	41096	144091	34.96%	4.513%
7	4.256	984	1000	1025	rBV2	57556	151612	36.78%	4.748%
8	4.963	1204	1220	1239	rBV2	128599	332635	80.70%	10.418%
9	5.539	1387	1399	1416	rBV	111303	236900	57.48%	7.419%
10	5.992	1527	1540	1554	rBV	74659	160118	38.85%	5.015%
11	6.445	1670	1681	1692	rBV8	2827	5782	1.40%	0.181%
12	6.921	1813	1829	1863	rBV	34001	76451	18.55%	2.394%
13	7.249	1920	1931	1958	rBV	148355	291851	70.81%	9.140%
14	7.561	2020	2028	2055	rBV3	18690	39777	9.65%	1.246%
15	7.911	2118	2137	2154	rVB4	21880	52903	12.84%	1.657%
16	8.030	2160	2174	2202	rBV	194068	412175	100.00%	12.909%
17	8.178	2212	2220	2235	rVB6	6965	14370	3.49%	0.450%
18	8.789	2397	2410	2440	rBV	186817	332007	80.55%	10.398%
19	10.159	2823	2836	2851	rBV	63392	104486	25.35%	3.272%
20	10.326	2877	2888	2901	rBV3	10563	17593	4.27%	0.551%
21	11.188	3143	3156	3176	rBV	190393	301971	73.26%	9.457%
22	11.564	3261	3273	3291	rBV	162352	260364	63.17%	8.154%
23	12.197	3461	3470	3480	rBV3	3513	6389	1.55%	0.200%




Sum of corrected areas: 3192965

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032399.D
Acq On : 11 Oct 2023 17:31
Operator : SY/MD
Sample : 04851-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

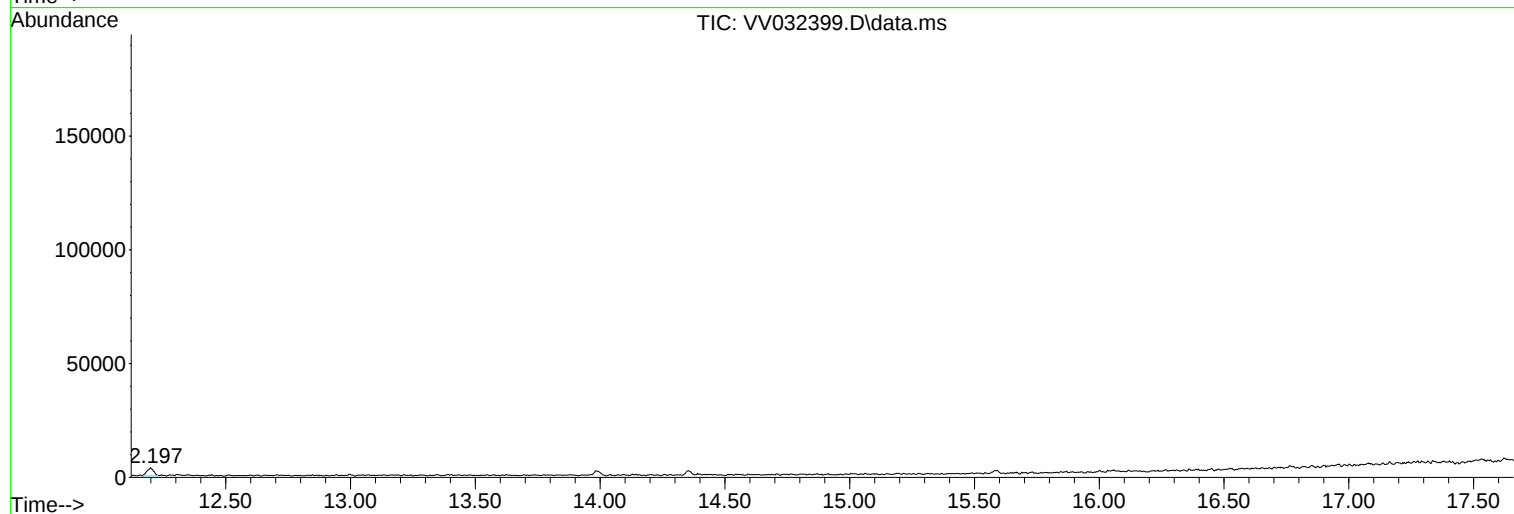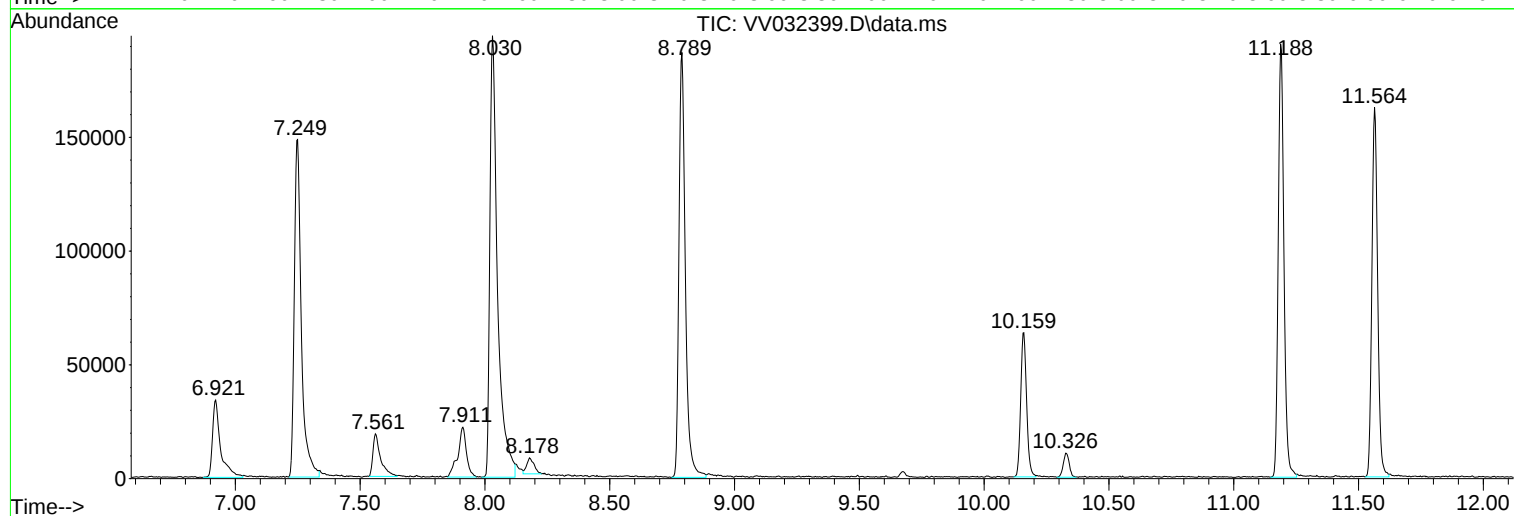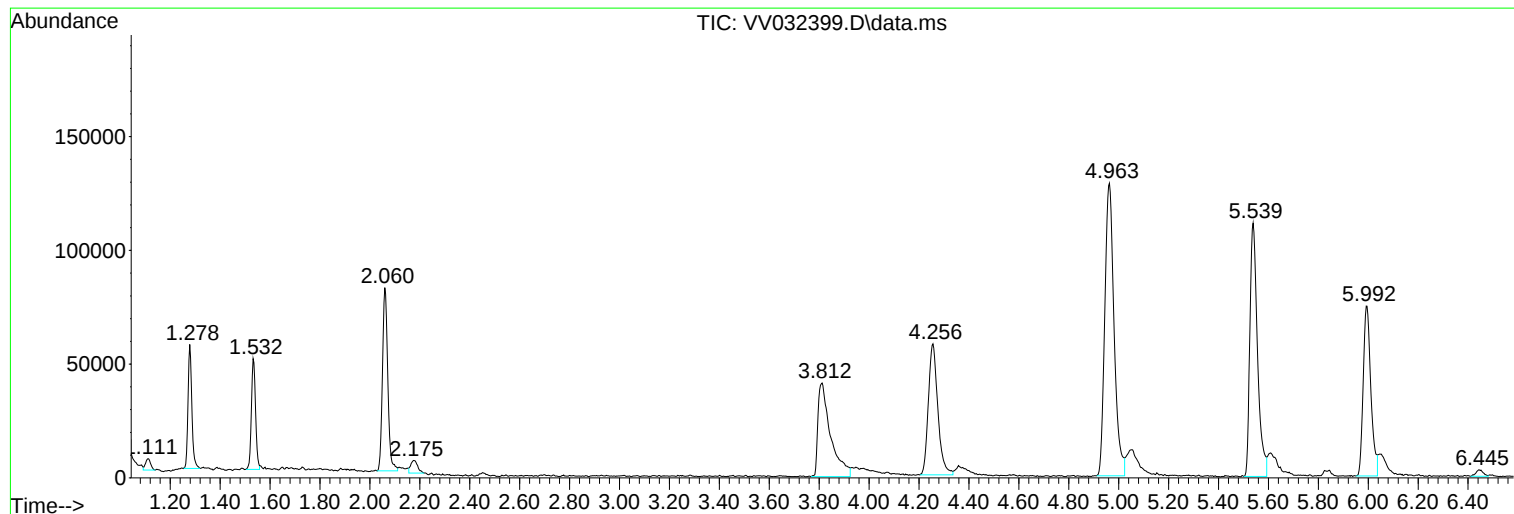

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032399.D
Acq On : 11 Oct 2023 17:31
Operator : SY/MD
Sample : 04851-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032399.D
Acq On : 11 Oct 2023 17:31
Operator : SY/MD
Sample : 04851-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc