

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
 Data File : VV032401.D
 Acq On : 11 Oct 2023 18:20
 Operator : SY/MD
 Sample : 04774-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	32	rVB	5423	7306	1.74%	0.228%
2	1.278	67	74	86	rBV	57375	60304	14.33%	1.884%
3	1.535	145	154	163	rBV	49526	58509	13.90%	1.828%
4	2.060	306	317	330	rBV	86437	126453	30.05%	3.951%
5	2.175	347	353	365	rVB	5953	10348	2.46%	0.323%
6	2.452	429	439	451	rBV4	4814	8991	2.14%	0.281%
7	3.812	853	862	892	rBV	39750	141701	33.67%	4.428%
8	4.252	983	999	1023	rBV2	58485	154929	36.82%	4.841%
9	4.963	1205	1220	1238	rBV3	134568	342244	81.33%	10.694%
10	5.538	1387	1399	1415	rBV	114421	240173	57.08%	7.504%
11	5.992	1527	1540	1555	rBV	76244	167275	39.75%	5.227%
12	6.921	1815	1829	1853	rBV	35256	75335	17.90%	2.354%
13	7.246	1919	1930	1959	rBV	157760	303811	72.20%	9.493%
14	7.561	2019	2028	2048	rBV2	20267	42606	10.13%	1.331%
15	7.879	2113	2127	2136	rBV2	5552	10205	2.43%	0.319%
16	8.030	2165	2174	2208	rBV	192767	420792	100.00%	13.148%
17	8.789	2395	2410	2437	rBV	189159	336853	80.05%	10.525%
18	10.159	2825	2836	2849	rBV	64629	104877	24.92%	3.277%
19	10.329	2879	2889	2898	rBV4	6719	9894	2.35%	0.309%
20	11.188	3144	3156	3174	rBV	193972	309390	73.53%	9.667%
21	11.564	3261	3273	3293	rBV	164555	263526	62.63%	8.234%
22	12.197	3463	3470	3480	rVB4	3148	4891	1.16%	0.153%




Sum of corrected areas: 3200413

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032401.D
Acq On : 11 Oct 2023 18:20
Operator : SY/MD
Sample : 04774-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

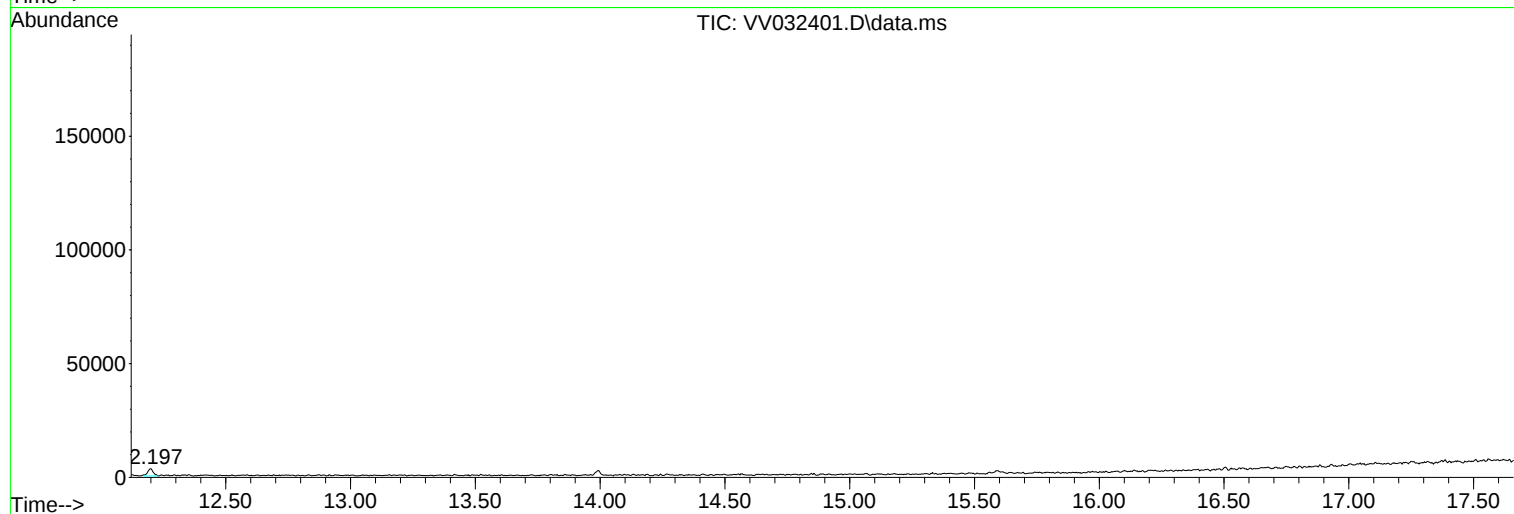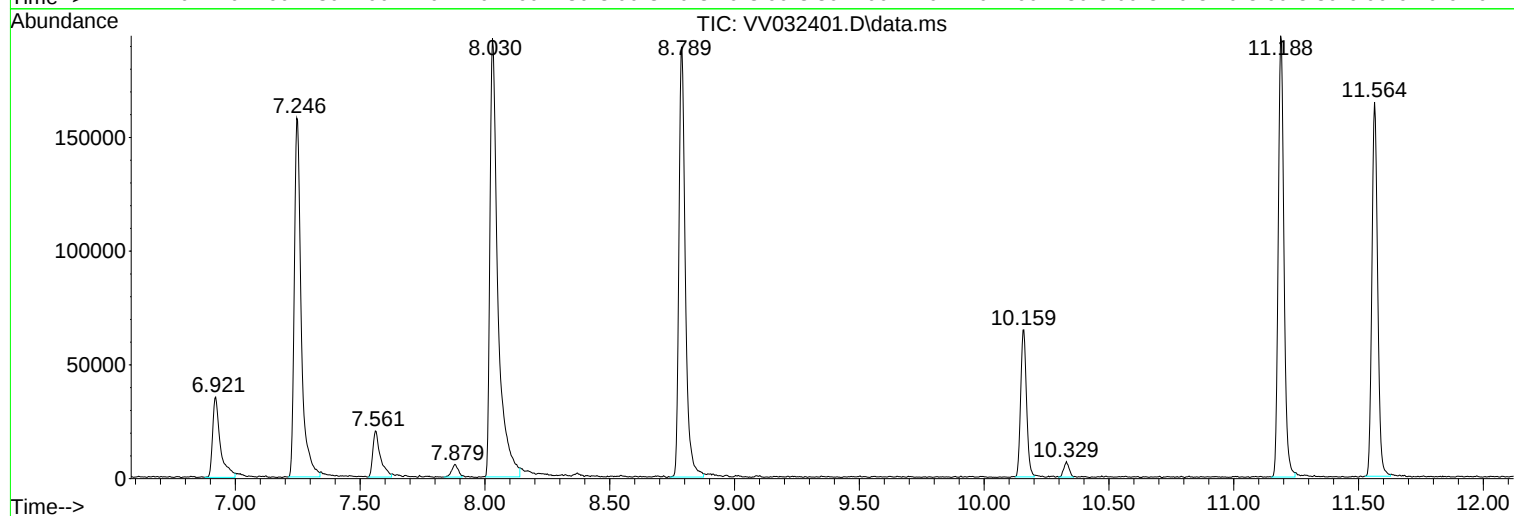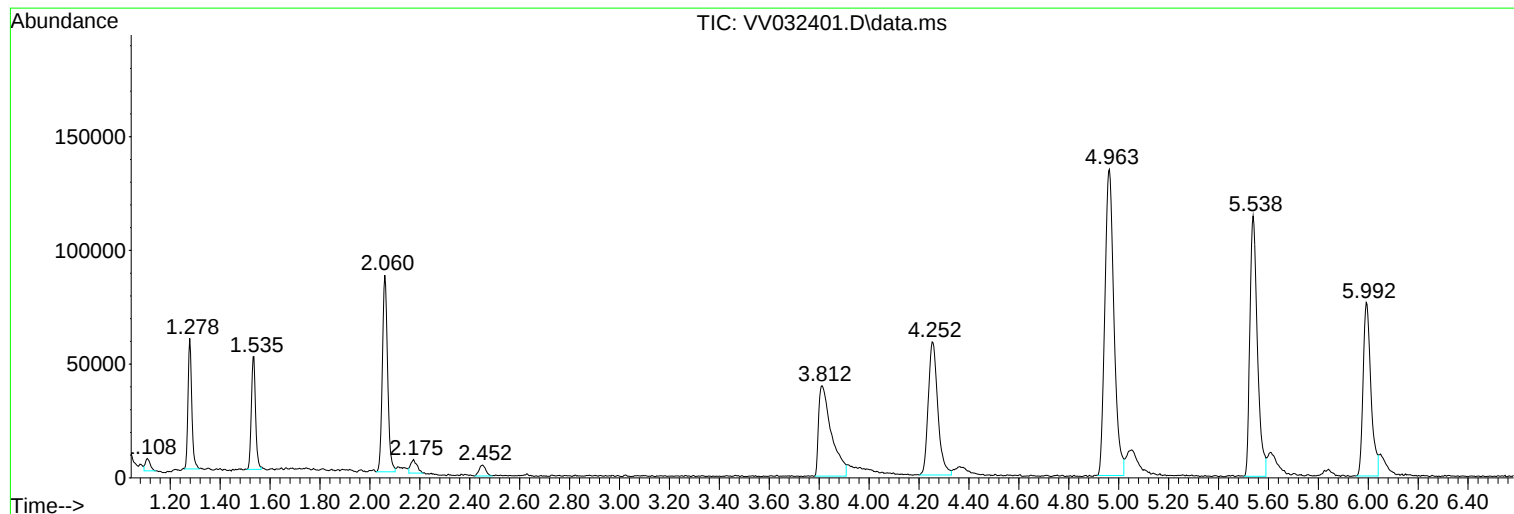

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032401.D
Acq On : 11 Oct 2023 18:20
Operator : SY/MD
Sample : 04774-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032401.D
Acq On : 11 Oct 2023 18:20
Operator : SY/MD
Sample : 04774-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc