
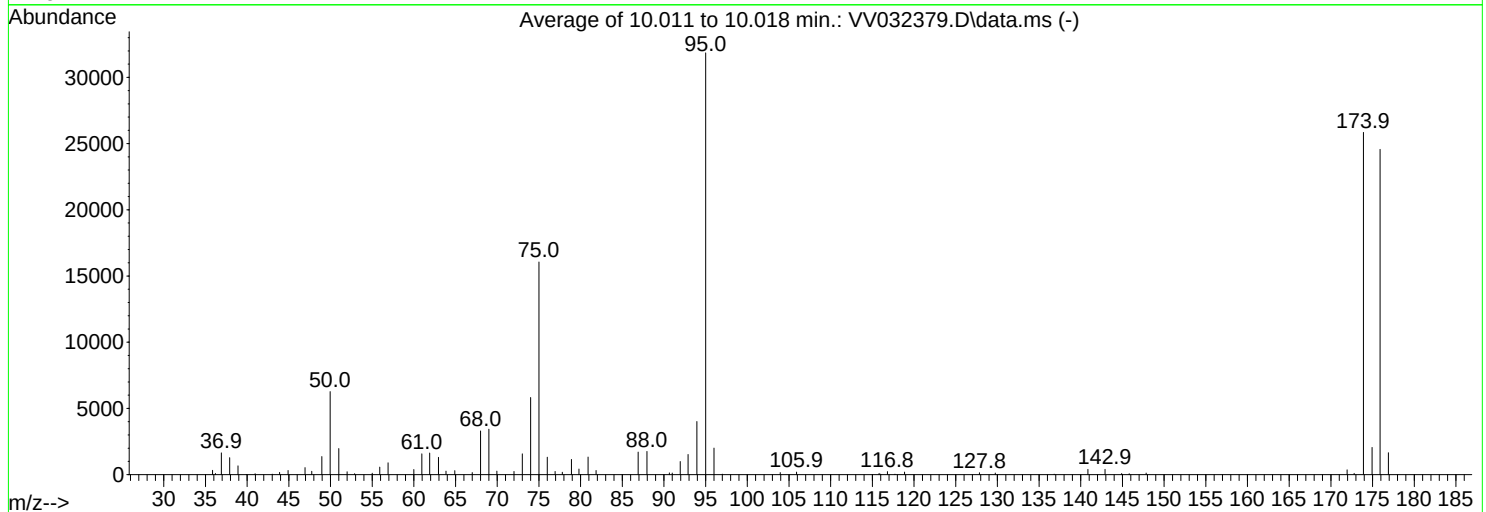


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101123\
Data File : VV032379.D
Acq On : 11 Oct 2023 08:46
Operator : SY/MD
Sample : BFB219
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB219

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Oct 12 02:54:58 2023

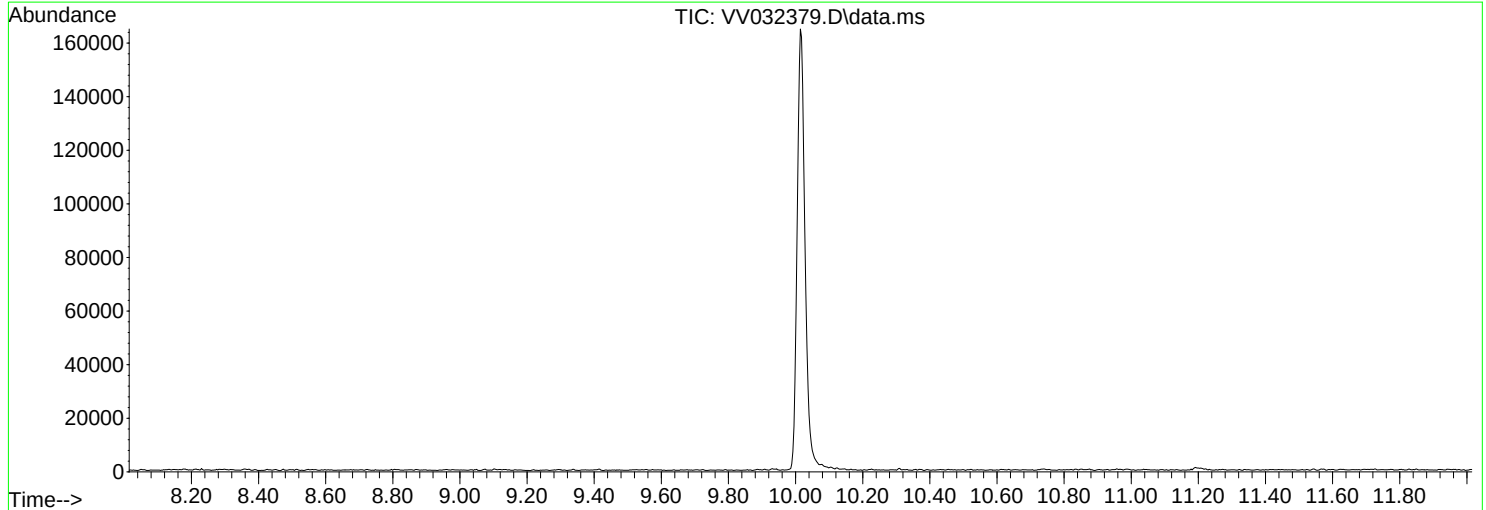

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	6277	PASS
75	95	30	80	50.4	16060	PASS
95	95	100	100	100.0	31851	PASS
96	95	5	9	6.3	2004	PASS
173	174	0.00	2	0.4	103	PASS
174	95	50	120	81.1	25843	PASS
175	174	5	9	7.9	2050	PASS
176	174	95	105	95.1	24568	PASS
177	176	5	10	6.8	1659	PASS

m/z	Abundance
38.50	109.0
39.90	322.0
43.90	345.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219

m/z	Abundance
35.80	305.0
36.20	274.0
36.90	1492.0
37.90	1256.0
38.90	665.0
39.90	334.0
43.90	499.0
44.90	355.0
47.00	598.0
47.80	241.0
48.90	1309.0
50.00	5901.0
51.00	1913.0
52.00	189.0
55.90	559.0
56.90	849.0
60.00	407.0
60.90	1539.0
61.90	1682.0
62.90	1299.0
63.90	275.0
64.90	243.0
67.10	152.0
68.00	3159.0
69.00	3260.0
69.90	301.0
72.00	248.0
73.00	1646.0
74.00	5619.0
75.00	15694.0
76.00	1360.0
76.90	281.0
77.80	168.0
78.90	1153.0
79.80	459.0
80.90	1224.0
81.90	289.0
86.90	1671.0
87.90	1636.0
90.70	113.0
91.00	114.0
91.90	929.0
92.90	1521.0
94.00	3728.0
95.00	30008.0
96.00	1986.0
103.90	146.0
105.90	197.0
115.80	166.0
116.80	232.0
118.90	177.0
127.80	154.0
129.70	131.0
140.90	363.0
142.90	392.0
144.90	131.0
145.80	101.0
147.80	128.0
172.00	330.0
173.90	23880.0
175.00	1937.0
175.90	23112.0
176.90	1635.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219

m/z	Abundance
35.90	332.0
36.90	1732.0
37.90	1304.0
38.90	663.0
40.00	316.0
41.00	103.0
43.90	521.0
44.90	331.0
47.00	533.0
47.70	268.0
49.00	1377.0
49.90	6528.0
51.00	2029.0
52.00	247.0
52.90	116.0
55.00	159.0
55.90	595.0
56.90	925.0
60.00	391.0
60.90	1644.0
61.90	1706.0
62.90	1357.0
63.80	285.0
64.90	306.0
67.00	158.0
68.00	3373.0
69.00	3569.0
69.90	266.0
72.00	256.0
73.00	1616.0
74.00	6077.0
75.00	16584.0
76.00	1346.0
77.00	256.0
77.80	188.0
78.90	1176.0
79.80	444.0
80.90	1405.0
81.90	323.0
86.90	1759.0
87.90	1843.0
90.60	136.0
91.00	131.0
92.00	1043.0
92.90	1558.0
93.90	4162.0
95.00	32896.0
96.00	2107.0
104.00	168.0
105.90	208.0
115.80	135.0
116.80	234.0
118.90	204.0
127.80	146.0
129.80	126.0
136.80	107.0
140.90	409.0
142.90	407.0
144.90	111.0
145.80	104.0
147.80	122.0
172.00	373.0
173.90	26704.0
175.00	2103.0
175.90	25384.0
176.90	1724.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219

m/z	Abundance
35.90	336.0
36.90	1694.0
37.90	1287.0
38.90	668.0
40.00	351.0
40.90	100.0
43.00	100.0
43.90	524.0
44.90	277.0
46.90	455.0
47.70	250.0
49.00	1403.0
50.00	6402.0
51.00	1962.0
52.00	202.0
52.90	110.0
55.00	181.0
55.90	558.0
56.90	922.0
60.00	349.0
61.00	1529.0
61.90	1515.0
63.00	1261.0
63.80	256.0
64.90	347.0
66.90	148.0
68.00	3352.0
69.00	3450.0
70.00	236.0
72.00	219.0
73.00	1464.0
74.00	5797.0
75.00	15902.0
76.00	1241.0
77.00	192.0
77.80	176.0
78.90	1108.0
79.80	357.0
80.90	1360.0
81.80	317.0
86.90	1674.0
88.00	1767.0
90.60	163.0
91.00	132.0
92.00	1003.0
92.90	1480.0
93.90	4136.0
95.00	32648.0
96.00	1919.0
97.00	109.0
104.00	161.0
105.90	171.0
116.00	129.0
116.80	240.0
117.70	109.0
118.80	214.0
127.90	133.0
129.80	124.0
140.80	420.0
142.90	416.0
147.90	113.0
171.90	387.0
172.80	308.0
173.90	26944.0
174.90	2110.0
175.90	25208.0
176.90	1617.0

Instrument :
MSVOA_V
ClientSampleId :
BFB219