

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101220\
 Data File : VV018855.D
 Acq On : 12 Oct 2020 14:43
 Operator : SY/MD
 Sample : L4289-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	83	rVB	250079	251674	17.16%	2.447%
2	1.576	144	151	166	rVB	192289	212282	14.47%	2.064%
3	2.119	310	320	345	rVB	378678	570530	38.89%	5.547%
4	2.618	472	475	476	rBV	310	165	0.01%	0.002%
5	2.737	508	512	514	rBV3	413	275	0.02%	0.003%
6	2.782	514	526	544	rVB3	7874	17502	1.19%	0.170%
7	2.868	549	553	555	rBV3	382	238	0.02%	0.002%
8	2.891	558	560	562	rBV	300	144	0.01%	0.001%
9	2.920	566	569	572	rVB2	288	177	0.01%	0.002%
10	2.939	572	575	579	rVB2	199	179	0.01%	0.002%
11	2.962	579	582	588	rBV2	754	775	0.05%	0.008%
12	3.000	590	594	596	rBV2	267	217	0.01%	0.002%
13	3.036	603	605	606	rBV2	259	107	0.01%	0.001%
14	3.045	606	608	609	rVV	451	171	0.01%	0.002%
15	3.058	610	612	617	rVB3	717	569	0.04%	0.006%
16	3.196	654	655	656	rBV3	132	41	0.00%	0.000%
17	3.209	658	659	662	rVB	163	45	0.00%	0.000%
18	3.235	663	667	669	rBV	238	138	0.01%	0.001%
19	3.248	669	671	673	rBV	147	77	0.01%	0.001%
20	3.290	680	684	685	rBV	113	49	0.00%	0.000%
21	3.296	685	686	691	rVV	328	245	0.02%	0.002%
22	3.331	691	697	702	rBV3	339	354	0.02%	0.003%
23	3.405	718	720	725	rVB	200	154	0.01%	0.001%
24	3.428	725	727	728	rBV	193	71	0.00%	0.001%
25	3.470	736	740	743	rBV2	256	259	0.02%	0.003%
26	3.563	764	769	770	rBV	474	355	0.02%	0.003%
27	3.602	778	781	783	rBV	183	128	0.01%	0.001%
28	3.640	789	793	794	rBV	371	286	0.02%	0.003%
29	3.676	800	804	806	rBV2	379	292	0.02%	0.003%
30	3.714	813	816	817	rBV	246	133	0.01%	0.001%
31	3.753	823	828	830	rBV	153	137	0.01%	0.001%
32	3.769	830	833	834	rBV2	212	128	0.01%	0.001%
33	3.798	840	842	845	rVB	366	176	0.01%	0.002%
34	3.856	855	860	862	rVB	214	166	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101220\
 Data File : VV018855.D
 Acq On : 12 Oct 2020 14:43
 Operator : SY/MD
 Sample : L4289-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

35	3.904	864	875	877	rBV	107320	172049	11.73%	1.673%
36	4.370	1003	1020	1050	rBV	221360	548451	37.39%	5.332%
37	4.630	1099	1101	1103	rBV2	257	156	0.01%	0.002%
38	4.669	1111	1113	1114	rBV2	356	168	0.01%	0.002%
39	4.817	1155	1159	1161	rBV2	335	219	0.01%	0.002%
40	4.881	1177	1179	1184	rVB2	337	147	0.01%	0.001%
41	4.907	1184	1187	1189	rVB	555	300	0.02%	0.003%
42	4.923	1190	1192	1195	rBV	284	155	0.01%	0.002%
43	4.939	1195	1197	1200	rBV	246	134	0.01%	0.001%
44	5.068	1220	1237	1268	rBV2	568737	1467019	100.00%	14.262%
45	5.415	1343	1345	1347	rBV2	280	115	0.01%	0.001%
46	5.486	1365	1367	1370	rBV2	513	272	0.02%	0.003%
47	5.637	1402	1414	1444	rBV	360475	734112	50.04%	7.137%
48	5.926	1493	1504	1527	rVB2	39104	84007	5.73%	0.817%
49	6.023	1531	1534	1535	rBV2	372	202	0.01%	0.002%
50	6.090	1539	1555	1582	rBV	307853	626719	42.72%	6.093%
51	6.367	1638	1641	1643	rBV2	473	327	0.02%	0.003%
52	6.405	1650	1653	1655	rBV2	304	194	0.01%	0.002%
53	6.540	1692	1695	1698	rBV	228	185	0.01%	0.002%
54	6.560	1698	1701	1703	rVV	274	189	0.01%	0.002%
55	6.576	1704	1706	1711	rVV2	421	300	0.02%	0.003%
56	6.611	1713	1717	1721	rVB3	432	379	0.03%	0.004%
57	6.627	1721	1722	1723	rBV3	141	48	0.00%	0.000%
58	6.656	1727	1731	1735	rBV2	201	231	0.02%	0.002%
59	6.717	1748	1750	1755	rBV2	442	321	0.02%	0.003%
60	6.756	1760	1762	1764	rBV	290	99	0.01%	0.001%
61	6.891	1803	1804	1806	rVB	219	58	0.00%	0.001%
62	6.907	1806	1809	1811	rBV2	189	130	0.01%	0.001%
63	6.926	1811	1815	1816	rBV	258	176	0.01%	0.002%
64	7.003	1825	1839	1862	rBV2	168411	314094	21.41%	3.054%
65	7.216	1903	1905	1906	rBV2	463	188	0.01%	0.002%
66	7.283	1924	1926	1928	rBV	305	145	0.01%	0.001%
67	7.335	1929	1942	1973	rBV	639123	1105902	75.38%	10.751%
68	7.640	2027	2037	2062	rBV	125158	218991	14.93%	2.129%
69	7.958	2131	2136	2142	rVB3	1310	1593	0.11%	0.015%
70	8.000	2142	2149	2158	rVB6	2290	3581	0.24%	0.035%
71	8.106	2172	2182	2222	rBV2	296261	620116	42.27%	6.029%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101220\
 Data File : VV018855.D
 Acq On : 12 Oct 2020 14:43
 Operator : SY/MD
 Sample : L4289-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

72	8.781	2389	2392	2395	rBV	487	361	0.02%	0.004%
73	8.871	2407	2420	2442	rBV	559261	899096	61.29%	8.741%
74	9.170	2510	2513	2516	rVB2	761	539	0.04%	0.005%
75	9.505	2612	2617	2620	rBV	393	381	0.03%	0.004%
76	9.531	2623	2625	2628	rBV	397	192	0.01%	0.002%
77	9.550	2629	2631	2636	rVB2	365	204	0.01%	0.002%
78	9.572	2636	2638	2639	rBV	410	201	0.01%	0.002%
79	9.688	2671	2674	2676	rBV	426	281	0.02%	0.003%
80	9.727	2683	2686	2693	rBV3	400	514	0.04%	0.005%
81	9.965	2757	2760	2764	rBV2	355	291	0.02%	0.003%
82	10.235	2832	2844	2863	rBV	348666	544252	37.10%	5.291%
83	10.405	2888	2897	2906	rBV3	1774	3243	0.22%	0.032%
84	10.473	2914	2918	2919	rBV	385	194	0.01%	0.002%
85	10.540	2937	2939	2944	rVB2	333	169	0.01%	0.002%
86	10.595	2954	2956	2958	rBV	361	209	0.01%	0.002%
87	10.736	2998	3000	3001	rBV	211	84	0.01%	0.001%
88	10.923	3056	3058	3061	rVB	292	143	0.01%	0.001%
89	10.942	3061	3064	3069	rBV3	421	374	0.03%	0.004%
90	11.006	3081	3084	3090	rBV	410	422	0.03%	0.004%
91	11.186	3138	3140	3144	rBV2	535	263	0.02%	0.003%
92	11.270	3155	3166	3188	rBV	552469	855939	58.35%	8.321%
93	11.473	3225	3229	3230	rBV2	545	404	0.03%	0.004%
94	11.646	3271	3283	3306	rBV	649526	1018072	69.40%	9.898%
95	11.891	3356	3359	3361	rBV2	360	249	0.02%	0.002%
96	11.955	3376	3379	3381	rBV	392	201	0.01%	0.002%
97	12.395	3515	3516	3520	rBV	289	150	0.01%	0.001%


Sum of corrected areas: 10286139

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101220\
Data File : VV018855.D
Acq On : 12 Oct 2020 14:43
Operator : SY/MD
Sample : L4289-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

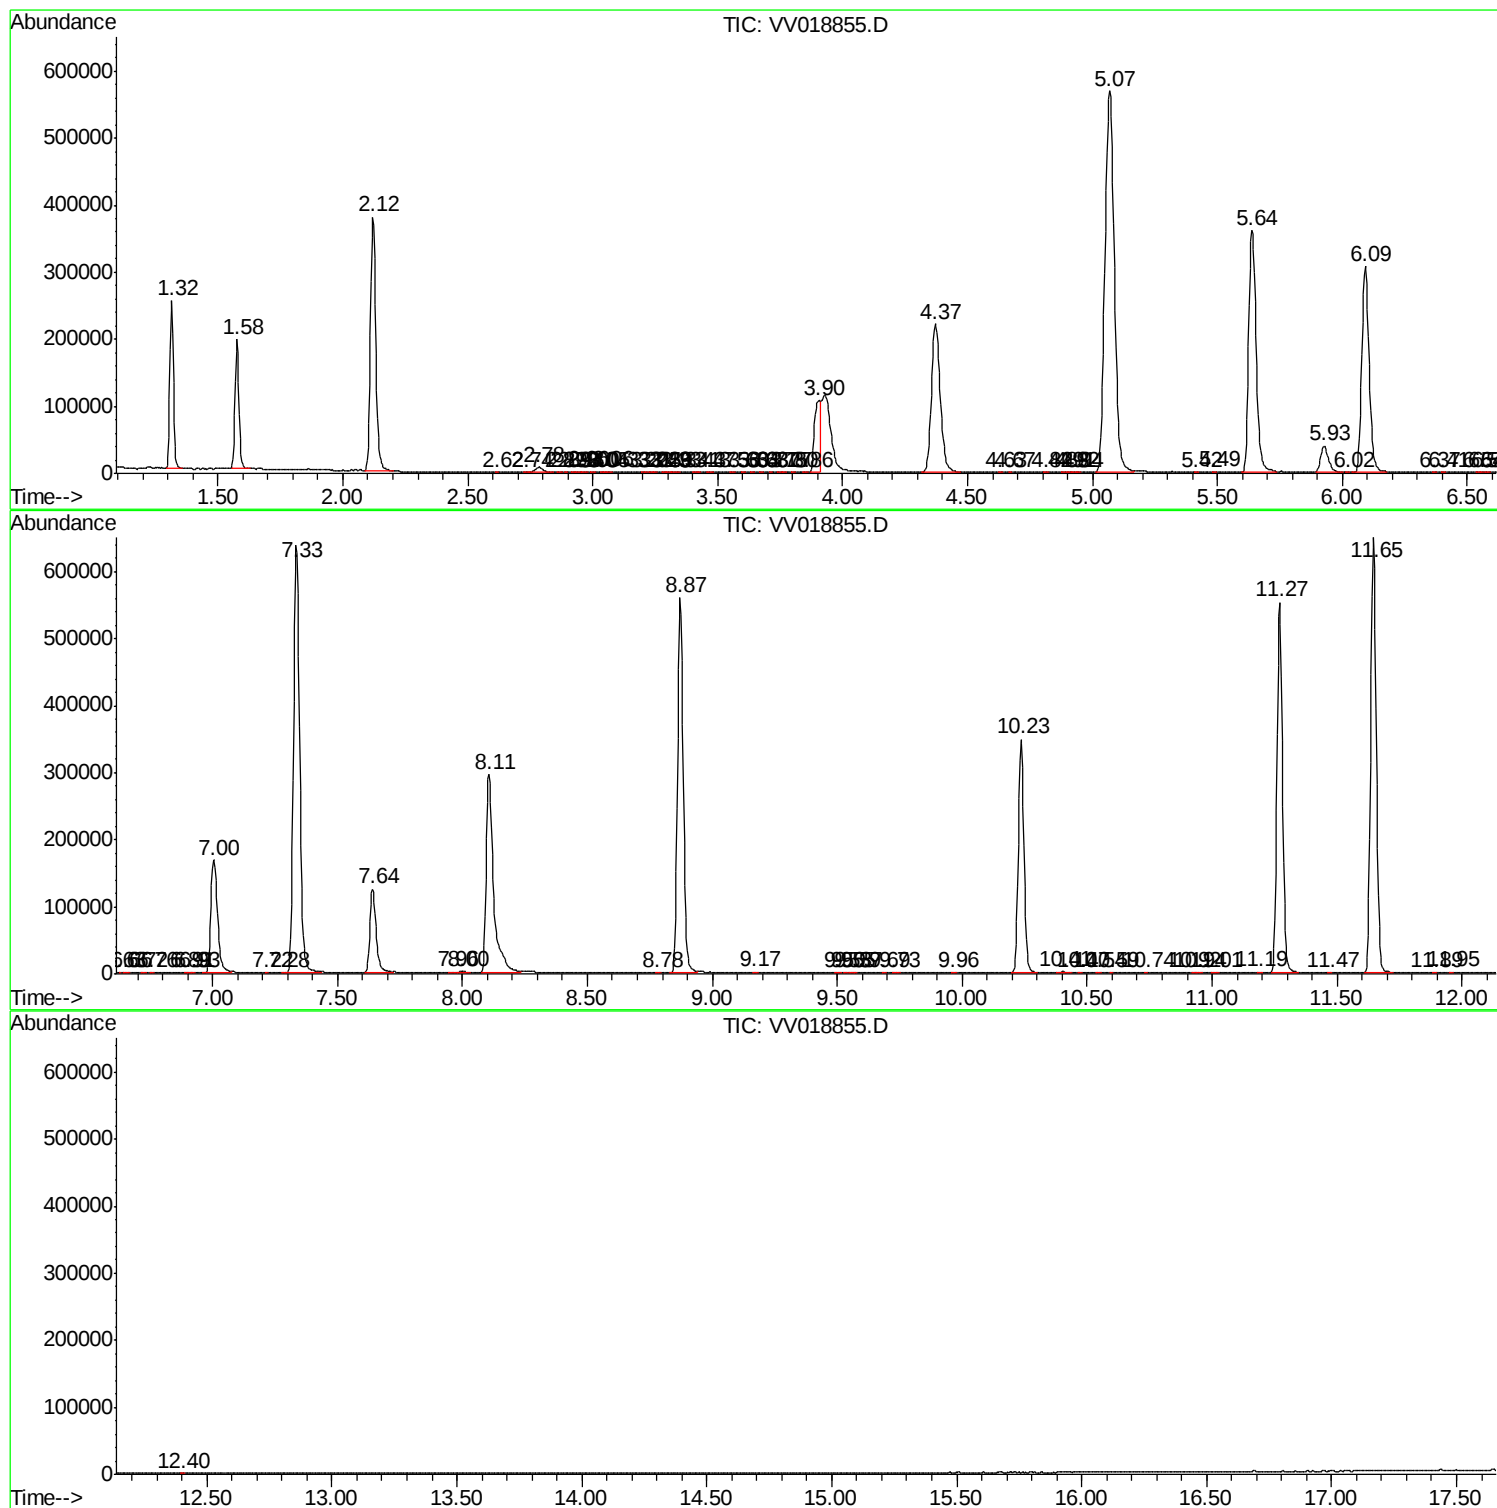

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV101220\
Data File : VV018855.D
Acq On : 12 Oct 2020 14:43
Operator : SY/MD
Sample : L4289-03
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AB6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV101220\
Data File : VV018855.D
Acq On : 12 Oct 2020 14:43
Operator : SY/MD
Sample : L4289-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc