


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV101220\
Data File : VV018848.D
Acq On : 12 Oct 2020 08:44
Operator : SY/MD
Sample : BFB72
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB72

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Title : VOC Analysis
Last Update : Thu Oct 15 16:44:05 2020

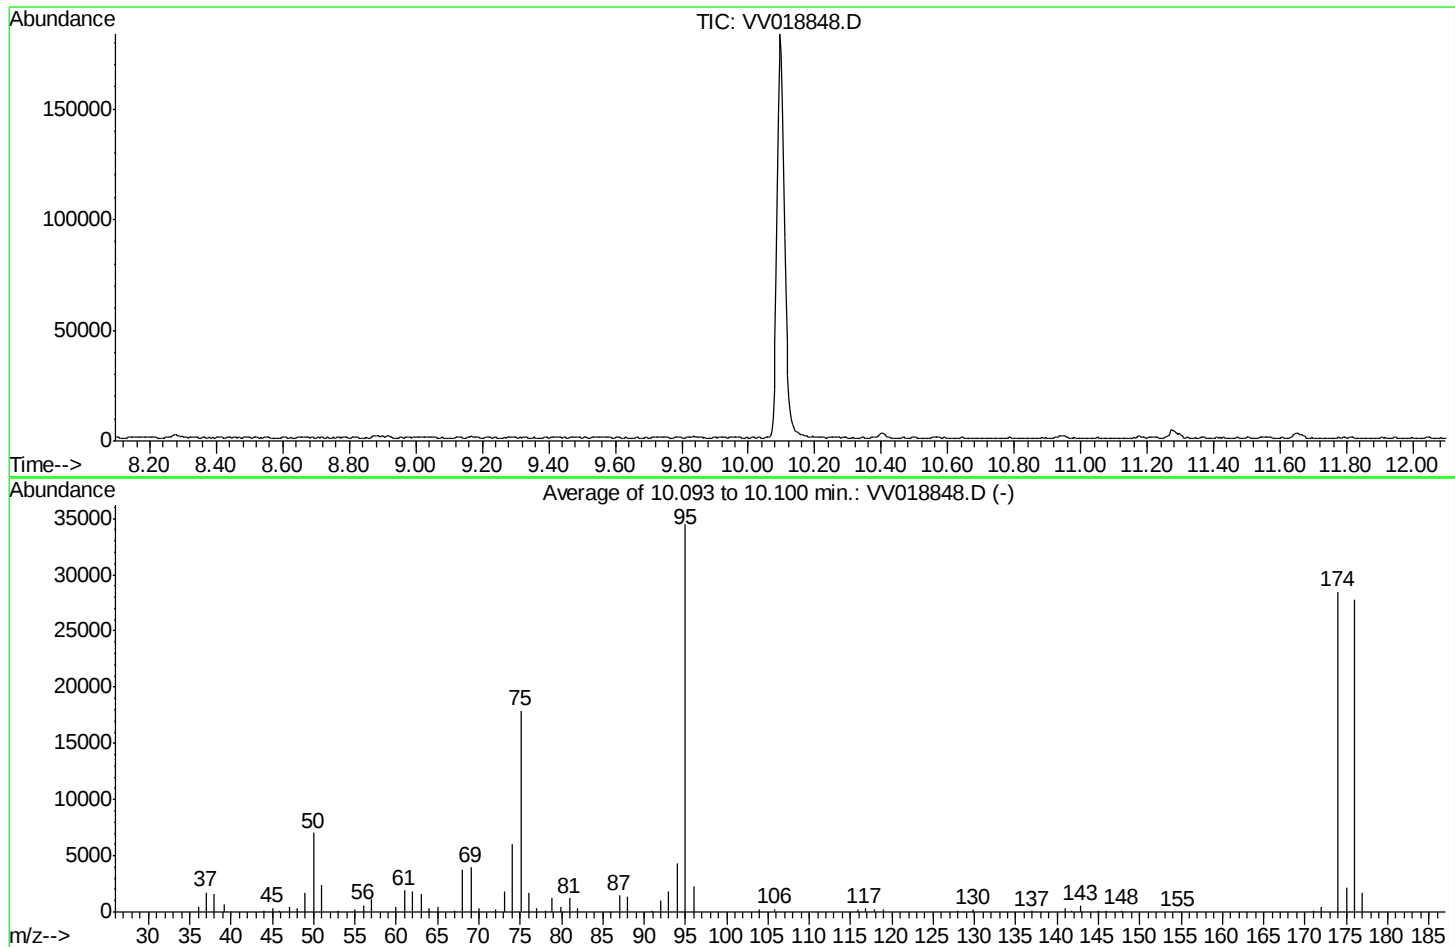

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	7030	PASS
75	95	30	80	51.9	17898	PASS
95	95	100	100	100.0	34482	PASS
96	95	5	9	6.7	2300	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.7	28512	PASS
175	174	5	9	7.5	2149	PASS
176	174	95	101	97.5	27789	PASS
177	176	5	9	6.4	1768	PASS

m/z	Abundance
36.00	418.0
37.00	1777.0
38.00	1648.0
39.10	708.0
39.90	401.0
44.00	1286.0
45.00	403.0
47.00	416.0
48.00	380.0
49.00	1811.0
50.00	6949.0
51.00	2383.0
53.00	114.0
55.00	227.0
56.00	569.0
57.00	1108.0
60.00	400.0
61.00	1848.0
62.00	1759.0
63.00	1657.0
64.00	331.0
65.00	467.0
67.00	142.0
68.00	3717.0
69.00	3970.0
70.10	308.0
72.00	294.0
73.10	1762.0
74.00	5863.0
75.10	17776.0
76.10	1712.0
77.00	259.0
78.00	113.0
78.90	1365.0
79.90	444.0
81.00	1201.0
81.90	347.0
85.80	102.0
87.00	1458.0
88.00	1442.0
90.90	144.0
92.00	1073.0
93.00	1869.0
94.10	4354.0
95.00	33640.0
96.00	2226.0
103.90	192.0
105.80	262.0
115.90	161.0
116.80	273.0
117.90	223.0
118.90	193.0
127.90	139.0
129.90	172.0
140.90	353.0
142.90	598.0
144.90	144.0
145.90	106.0
147.90	108.0
171.90	460.0
174.00	27200.0
175.00	2219.0
176.00	26464.0
177.00	1683.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
36.00	420.0
37.00	1799.0
38.00	1705.0
39.10	734.0
40.00	337.0
44.00	1261.0
45.00	353.0
45.80	121.0
47.10	416.0
48.00	386.0
49.00	1811.0
50.00	7257.0
51.00	2418.0
53.00	106.0
55.00	174.0
56.00	622.0
57.00	1208.0
59.90	494.0
61.00	1939.0
62.00	1910.0
63.10	1681.0
64.00	332.0
65.00	518.0
67.00	152.0
68.00	3926.0
69.00	4151.0
70.00	306.0
72.00	267.0
73.00	1873.0
74.00	6222.0
75.00	18376.0
76.10	1737.0
77.00	311.0
77.90	124.0
78.90	1353.0
80.00	413.0
81.00	1306.0
81.90	358.0
87.00	1463.0
87.90	1451.0
90.90	151.0
92.00	1120.0
93.00	1965.0
94.10	4444.0
95.00	35800.0
96.00	2368.0
103.90	201.0
105.80	241.0
115.90	192.0
116.80	297.0
117.90	187.0
118.90	207.0
127.90	148.0
129.80	193.0
137.00	106.0
141.00	378.0
141.80	120.0
142.90	572.0
145.00	152.0
145.90	151.0
147.80	144.0
171.00	101.0
171.90	531.0
174.00	29520.0
175.00	2213.0
176.00	28768.0
177.00	1793.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
36.00	378.0
37.00	1680.0
38.00	1549.0
39.10	739.0
40.00	338.0
44.00	1300.0
45.00	293.0
45.80	131.0
47.10	381.0
48.00	300.0
49.00	1655.0
50.00	6886.0
51.00	2216.0
53.00	111.0
55.00	135.0
56.00	580.0
57.00	1103.0
59.90	482.0
61.00	1871.0
62.00	1764.0
63.10	1498.0
64.00	262.0
65.00	551.0
67.00	143.0
68.00	3739.0
69.00	3800.0
70.00	289.0
72.00	226.0
73.00	1789.0
74.10	5892.0
75.00	17544.0
76.10	1559.0
77.00	311.0
78.10	121.0
78.90	1211.0
80.00	388.0
80.90	1196.0
81.90	342.0
87.00	1424.0
87.90	1283.0
90.90	173.0
92.00	1026.0
93.00	1655.0
94.00	4247.0
95.00	34008.0
96.00	2308.0
103.90	166.0
105.90	195.0
115.90	196.0
116.80	305.0
117.90	156.0
118.90	237.0
127.90	150.0
128.80	105.0
129.90	186.0
137.00	101.0
141.00	423.0
141.80	111.0
142.90	470.0
145.00	160.0
145.90	166.0
147.80	144.0
154.70	107.0
171.10	115.0
172.00	519.0
174.00	28816.0
175.00	2015.0
176.00	28136.0
177.00	1829.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

Scan 2789 (10.058 min): VV018848.D
BFB72

m/z	Abundance
39.90	303.0
42.90	130.0
44.00	1165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72