

Quantitation Report (QT Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101221\
 Data File : VV022755.D
 Acq On : 12 Oct 2021 15:51
 Operator : SY/MD
 Sample : M4126-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC7

Quant Time: Oct 13 01:18:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 13 01:15:35 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 10/13/2021 8:23:39 AM

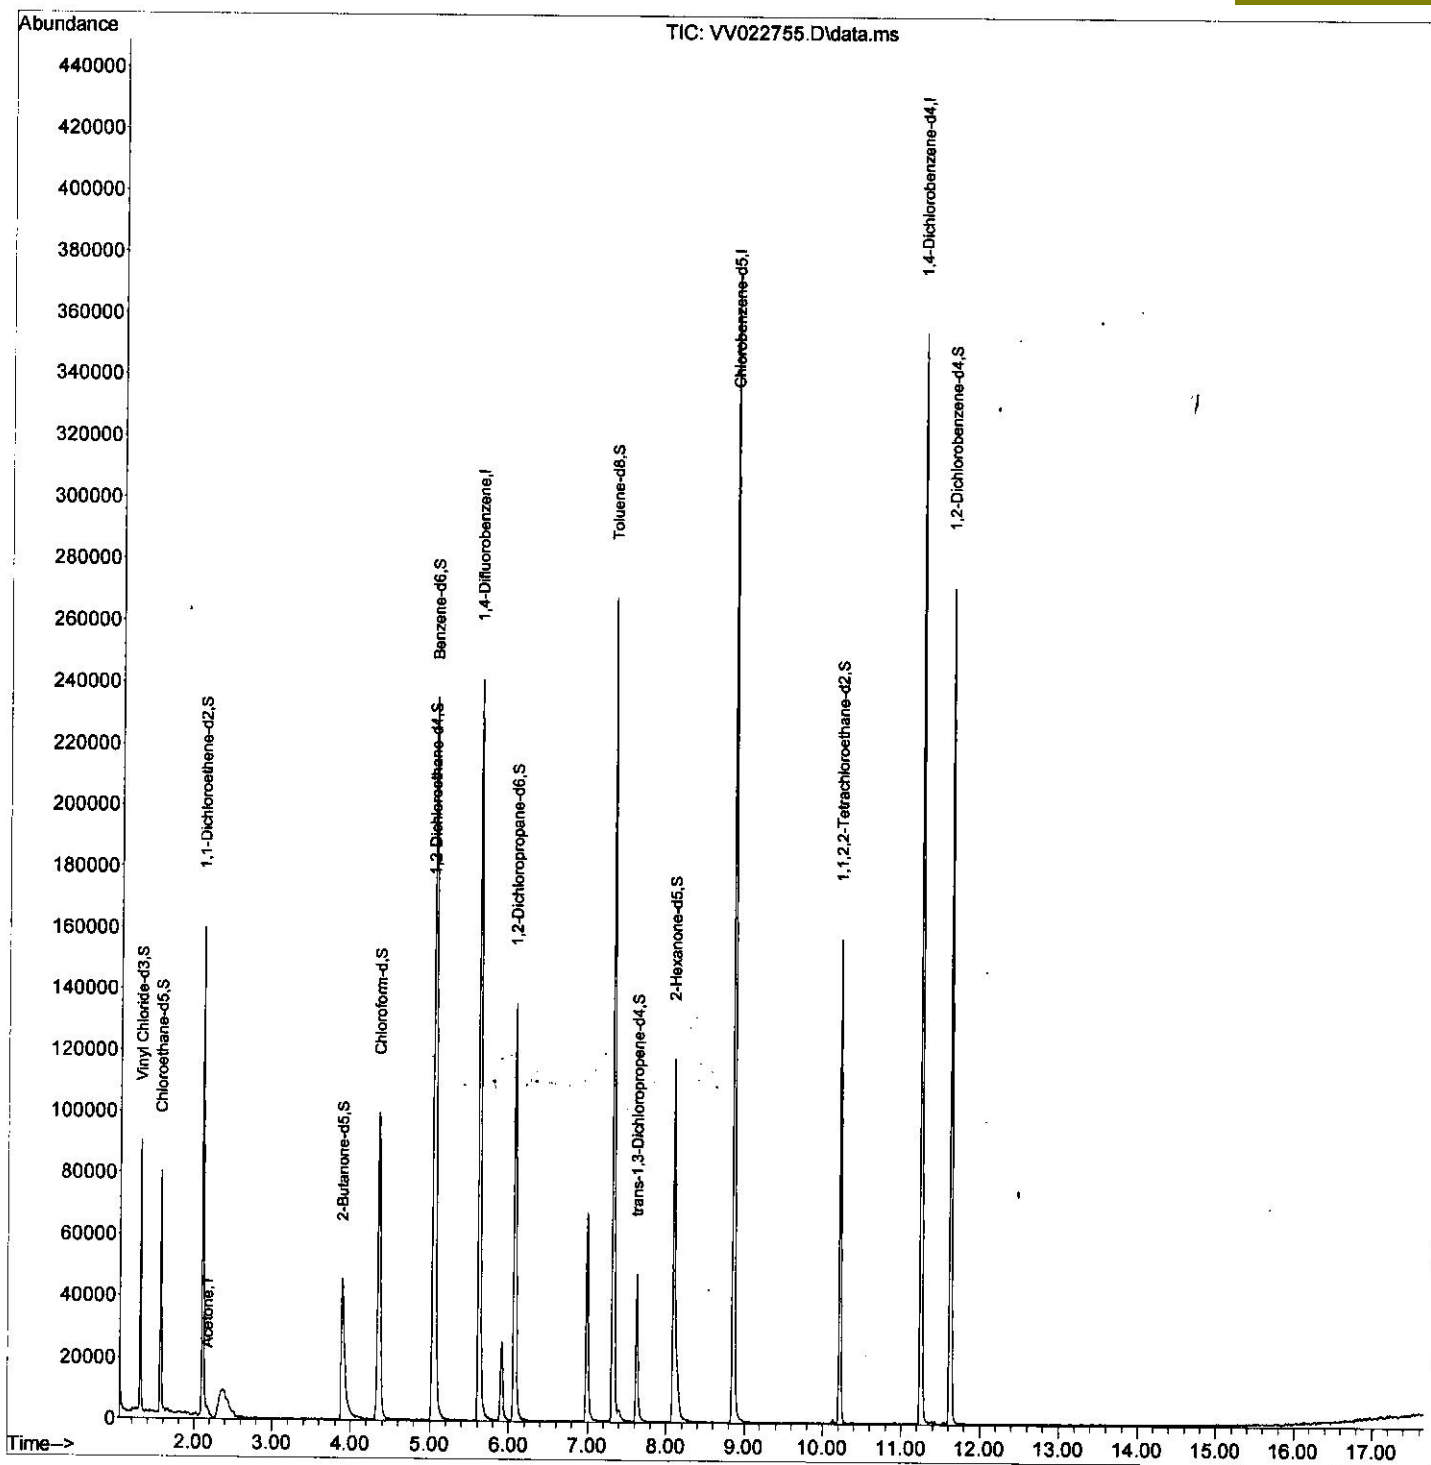

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101221\
 Data File : VV022755.D
 Acq On : 12 Oct 2021 15:51
 Operator : SY/MD
 Sample : M4126-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC7

Quant Time: Oct 13 01:18:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 13 01:15:35 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 10/13/2021 8:23:39 AM

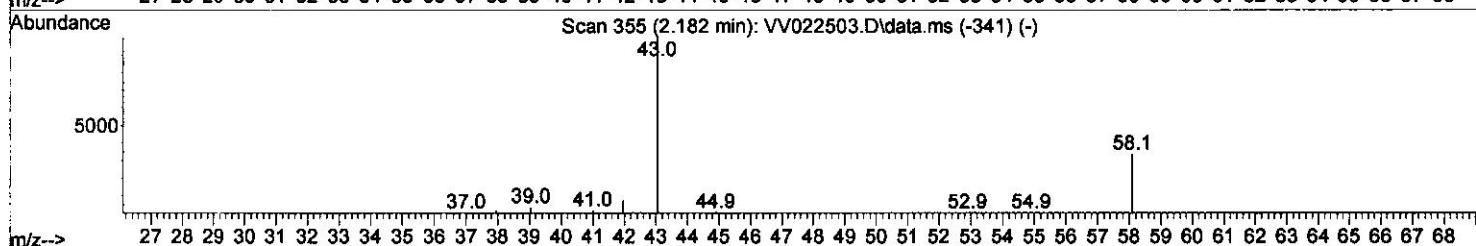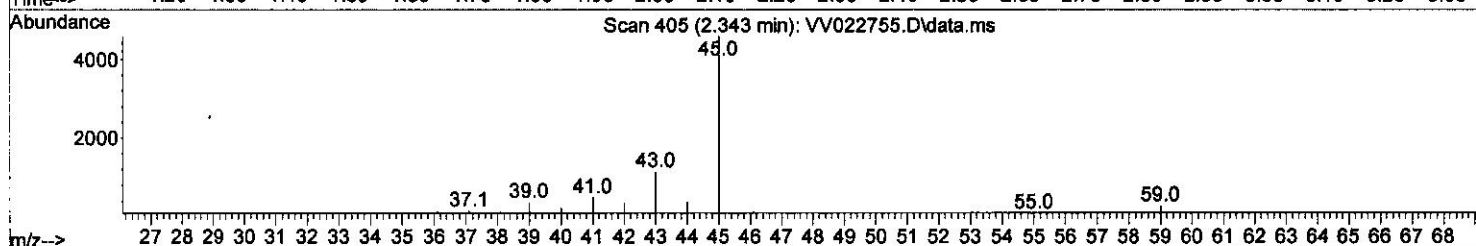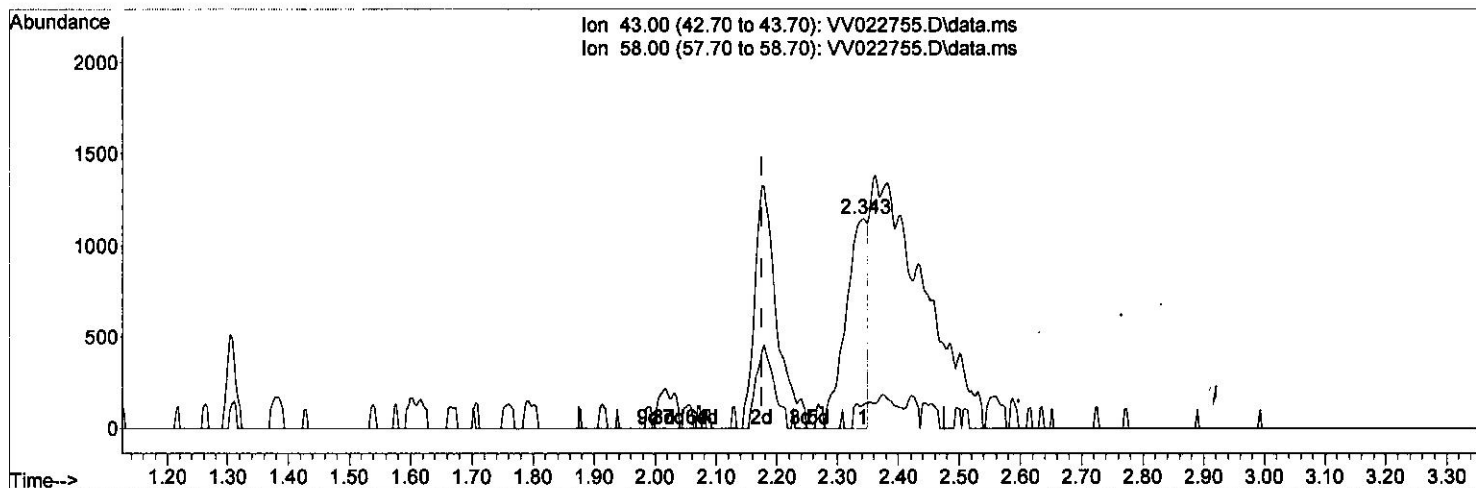

TIC: VV022755.D\data.ms

(13) Acetone (T)

2.343min (+ 0.167) 3.07 ug/L

response 2832

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	10.60	3.39
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101221\
 Data File : VV022755.D
 Acq On : 12 Oct 2021 15:51
 Operator : SY/MD
 Sample : M4126-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 C0AC7

Quant Time: Oct 13 01:18:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 13 01:15:35 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 10/13/2021 8:23:39 AM

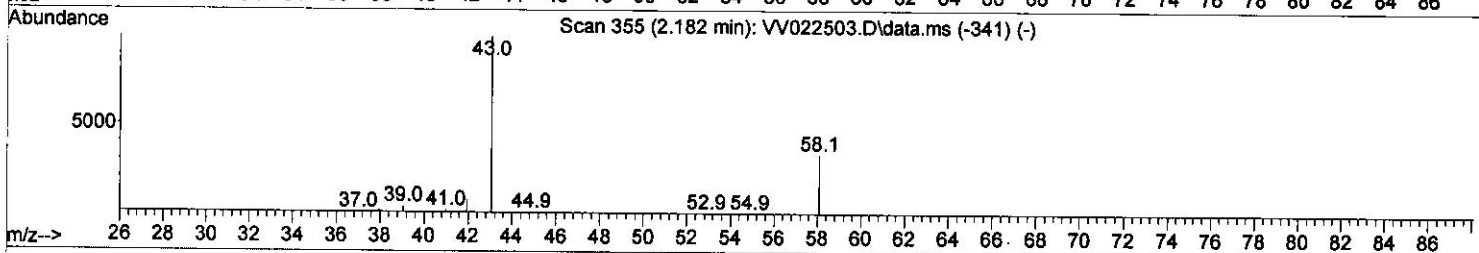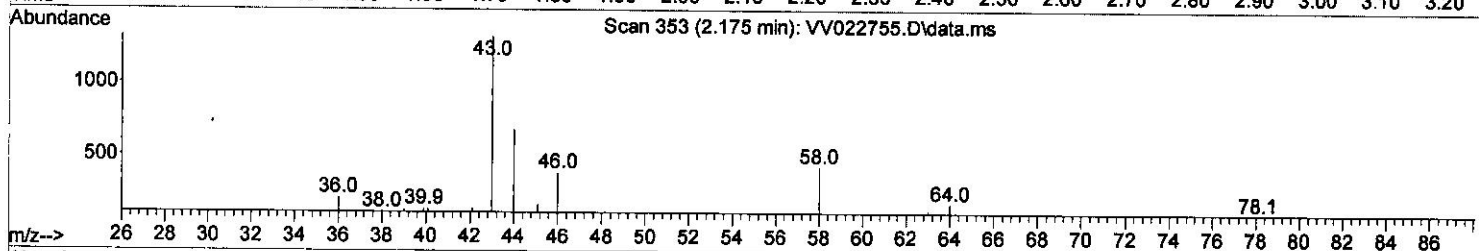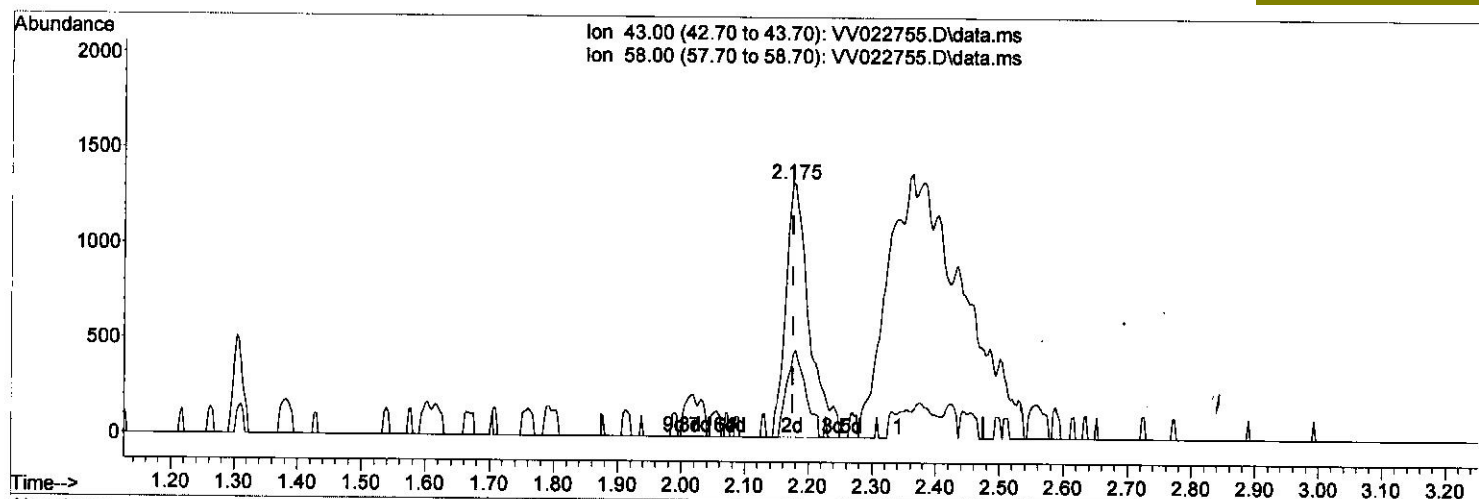

TIC: VV022755.D\data.ms

(13) Acetone (T)

2.175min (+ 0.000) 3.69 ug/L m *3 mp 10/22/21*

response 3406

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	10.60	2.82
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101221\
 Data File : VW022755.D
 Acq On : 12 Oct 2021 15:51
 Operator : SY/MD
 Sample : M4126-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC7

Quant Time: Oct 13 01:18:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 13 01:15:35 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 10/13/2021 8:23:39 AM

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	214706	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	210768	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	96026	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	54231	40.841	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	81.680%		
7) Chloroethane-d5	1.568	69	45570	43.658	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	87.320%		
11) 1,1-Dichloroethene-d2	2.108	63	80367	30.695	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	61.380%		
21) 2-Butanone-d5	3.889	46	76370	104.484	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	104.480%		
24) Chloroform-d	4.352	84	106652	43.961	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.920%		
26) 1,2-Dichloroethane-d4	5.034	65	64603	45.904	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.800%		
32) Benzene-d6	5.053	84	207738	42.545	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.080%		
36) 1,2-Dichloropropane-d6	6.072	67	66328	44.126	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.260%		
41) Toluene-d8	7.320	98	181398	40.500	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	81.000%		
43) trans-1,3-Dichloroprop...	7.625	79	27760	39.033	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.060%		
47) 2-Hexanone-d5	8.091	63	37786	60.682	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	60.680%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	73641	35.231	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	70.460%		
66) 1,2-Dichlorobenzene-d4	11.625	152	75347	48.116	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.240%		

Target Compounds

13) Acetone	2.175	43	3406m	3.689	ug/L	Qvalue
-------------	-------	----	-------	-------	------	--------

MD
 10/22/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed