

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101221\
 Data File : VW022751.D
 Acq On : 12 Oct 2021 14:10
 Operator : SY/MD
 Sample : M4126-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

apatel
 10/13/2021 8:23:43 AM

Quant Time: Oct 13 01:17:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 13 01:15:35 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	176378	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	170442	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	77964	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	55773	51.129	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	102.260%
7) Chloroethane-d5	1.565	69	44730	52.166	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	104.340%
11) 1,1-Dichloroethene-d2	2.108	63	79092	36.772	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.540%
21) 2-Butanone-d5	3.883	46	70012	116.600	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	116.600%
24) Chloroform-d	4.349	84	101966	51.163	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.320%
26) 1,2-Dichloroethane-d4	5.034	65	63420	54.856	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.720%
32) Benzene-d6	5.053	84	202515	51.288	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.580%
36) 1,2-Dichloropropane-d6	6.072	67	65483	53.870	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	107.740%
41) Toluene-d8	7.317	98	174924	48.295	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.600%
43) trans-1,3-Dichloroprop...	7.625	79	26842	46.672	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.340%
47) 2-Hexanone-d5	8.092	63	34074	67.667	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	67.670%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	69829	41.312	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	82.620%
66) 1,2-Dichlorobenzene-d4	11.625	152	68482	53.863	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.720%
Target Compounds					Qvalue	
13) Acetone	2.169	43	3393m	4.473	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101221\
Data File : VV022751.D
Acq On : 12 Oct 2021 14:10
Operator : SY/MD
Sample : M4126-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

apatel
10/13/2021 8:23:43 AM

Quant Time: Oct 13 01:17:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 13 01:15:35 2021
Response via : Initial Calibration

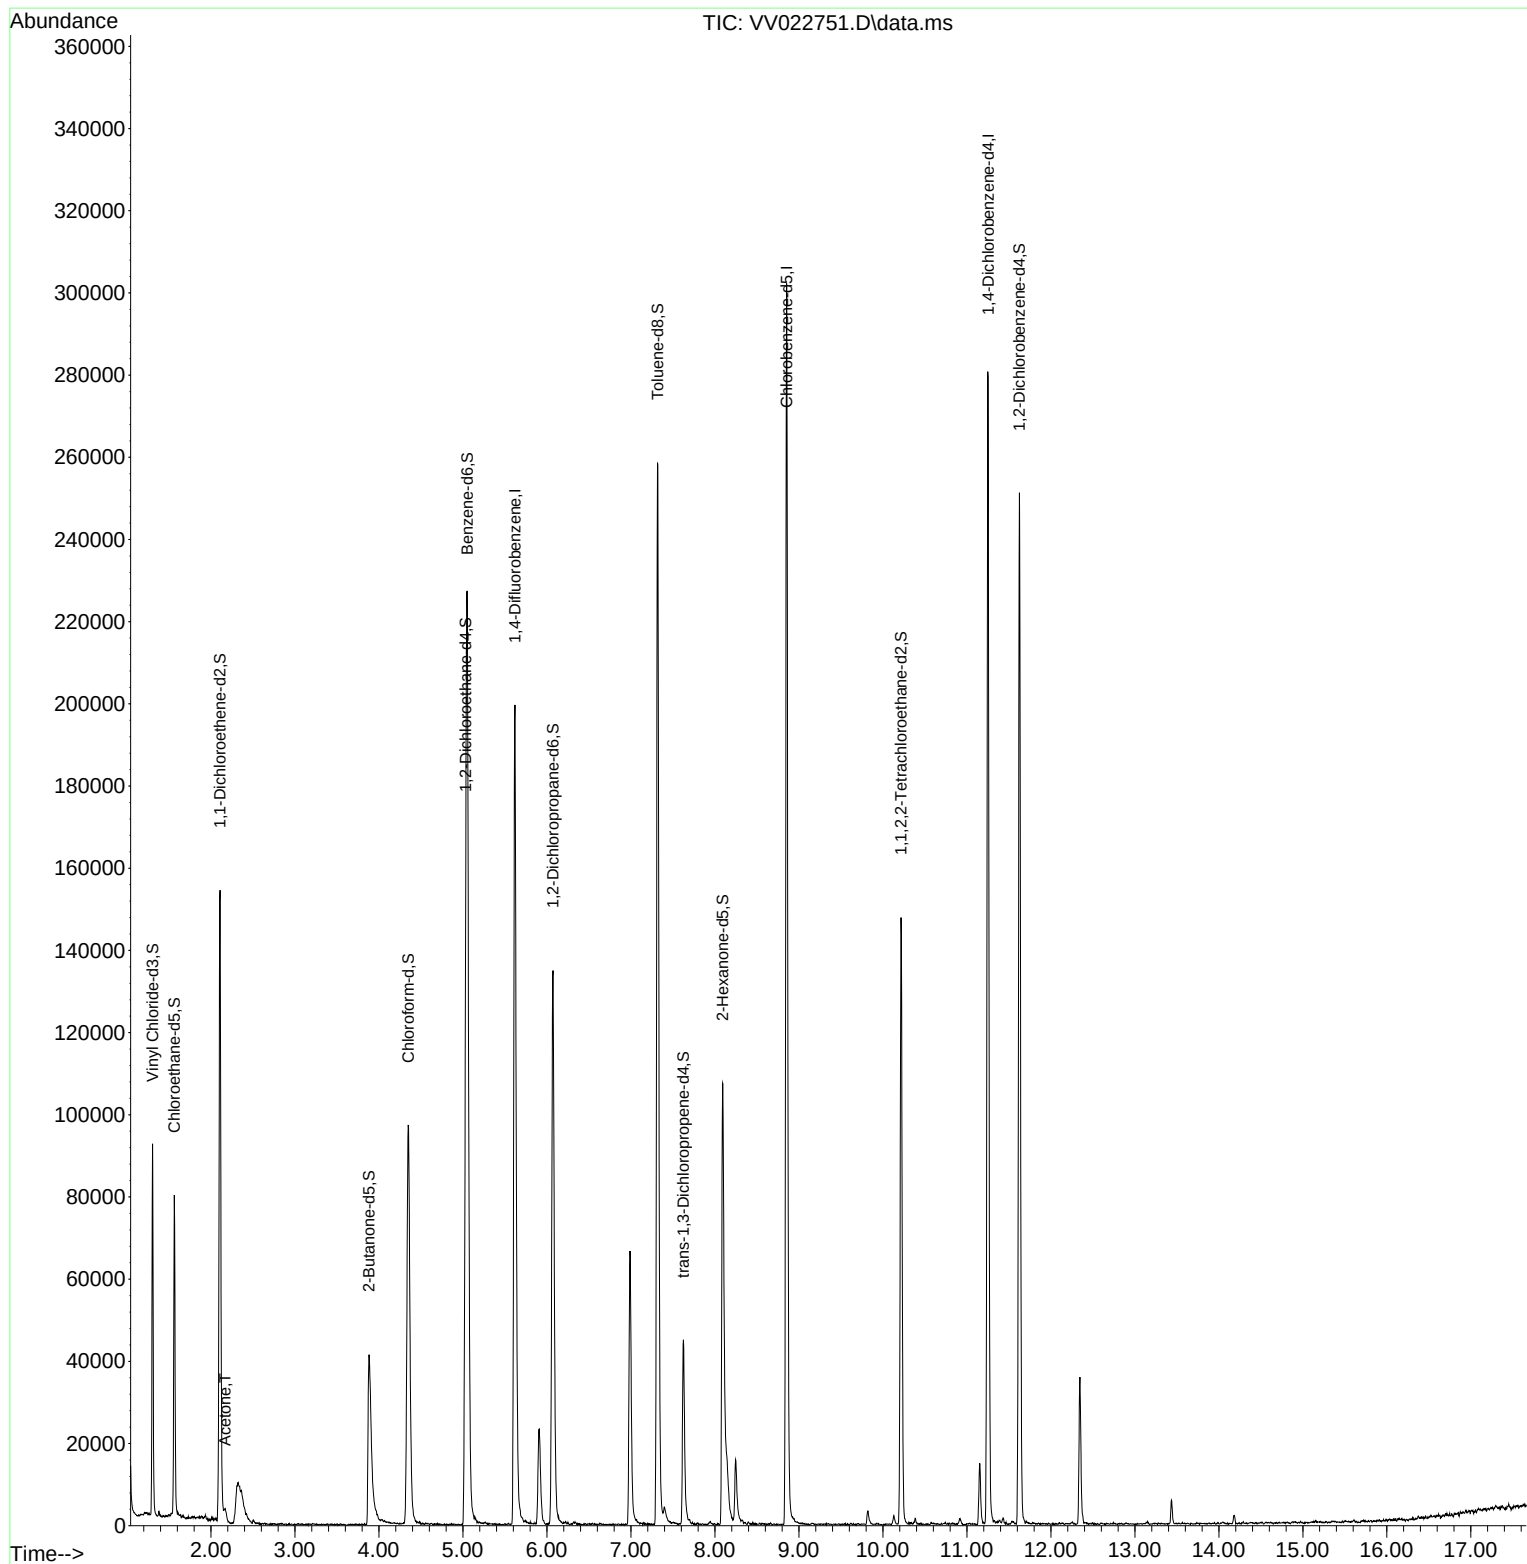

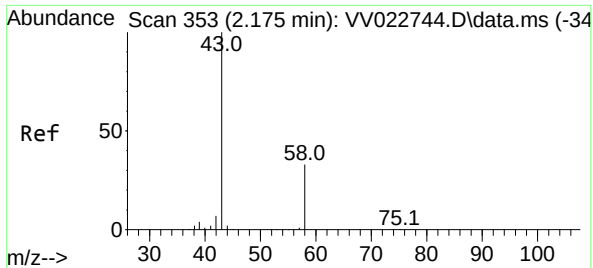

#13
Acetone
Concen: 4.473 ug/L m
RT: 2.169 min Scan# 351
Delta R.T. -0.006 min
Lab File: VV022751.D
Acq: 12 Oct 2021 14:10

Tgt Ion: 43 Resp: 3393
Ion Ratio Lower Upper
43 100
58 5.9 0.0 21.2

Instrument :
MSVOA_V
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

apatel
10/13/2021 8:23:43 AM

