

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101221\
 Data File : VV022753.D
 Acq On : 12 Oct 2021 14:58
 Operator : SY/MD
 Sample : M4125-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGB16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M

Title : VOC Analysis

Signal : TIC: VV022753.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	94	rVB	97097	97447	14.78%	1.757%
2	1.568	157	164	181	rVB	84608	105477	16.00%	1.902%
3	2.108	322	332	346	rBV	170089	252040	38.22%	4.545%
4	2.503	452	455	456	rBV	617	366	0.06%	0.007%
5	2.802	546	548	550	rBV	158	83	0.01%	0.001%
6	3.127	645	649	651	rBV	301	276	0.04%	0.005%
7	3.191	656	669	689	rVV	39334	81720	12.39%	1.474%
8	3.339	712	715	720	rBV2	229	250	0.04%	0.005%
9	3.359	720	721	722	rBV	366	108	0.02%	0.002%
10	3.404	733	735	736	rBV	222	81	0.01%	0.001%
11	3.886	875	885	919	rBV	49324	152947	23.19%	2.758%
12	4.349	1014	1029	1053	rBV	105783	267320	40.54%	4.821%
13	4.555	1091	1093	1097	rVB2	354	205	0.03%	0.004%
14	4.609	1097	1110	1132	rBV4	11589	28845	4.37%	0.520%
15	4.735	1148	1149	1150	rBV4	215	64	0.01%	0.001%
16	4.831	1177	1179	1182	rBV2	233	80	0.01%	0.001%
17	4.847	1182	1184	1186	rBV	181	71	0.01%	0.001%
18	4.918	1203	1206	1207	rBV	287	160	0.02%	0.003%
19	4.963	1218	1220	1221	rBV	363	177	0.03%	0.003%
20	5.050	1230	1247	1277	rBV2	254527	659407	100.00%	11.891%
21	5.452	1367	1372	1373	rBV2	366	301	0.05%	0.005%
22	5.516	1389	1392	1394	rBV	208	140	0.02%	0.003%
23	5.619	1412	1424	1448	rBV	258311	519700	78.81%	9.372%
24	5.912	1503	1515	1536	rBV5	22618	52044	7.89%	0.938%
25	6.008	1543	1545	1551	rVB3	451	308	0.05%	0.006%
26	6.072	1551	1565	1588	rBV	148778	304280	46.14%	5.487%
27	6.201	1603	1605	1607	rBV2	463	220	0.03%	0.004%
28	6.304	1633	1637	1638	rBV	401	229	0.03%	0.004%
29	6.513	1699	1702	1704	rBV2	279	176	0.03%	0.003%
30	6.571	1718	1720	1723	rVB3	347	166	0.03%	0.003%
31	6.680	1752	1754	1755	rBV3	276	139	0.02%	0.003%
32	6.722	1764	1767	1770	rBV	334	262	0.04%	0.005%
33	6.844	1801	1805	1809	rBV	370	324	0.05%	0.006%
34	6.989	1839	1850	1874	rBV	75356	140351	21.28%	2.531%
35	7.320	1940	1953	1970	rBV	292778	510956	77.49%	9.214%
36	7.625	2038	2048	2070	rBV2	52592	92640	14.05%	1.671%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101221\
 Data File : VV022753.D
 Acq On : 12 Oct 2021 14:58
 Operator : SY/MD
 Sample : M4125-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGB16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	7.899	2131	2133	2137	rVB	344	154	0.02%	0.003%
38	8.092	2183	2193	2230	rBV2	136737	287305	43.57%	5.181%
39	8.403	2289	2290	2292	rBV2	327	150	0.02%	0.003%
40	8.461	2302	2308	2311	rBV3	379	442	0.07%	0.008%
41	8.677	2373	2375	2377	rVB2	239	75	0.01%	0.001%
42	8.854	2419	2430	2462	rBV	393329	640595	97.15%	11.552%
43	9.085	2498	2502	2504	rBV	249	160	0.02%	0.003%
44	9.249	2551	2553	2555	rBV	241	76	0.01%	0.001%
45	9.313	2571	2573	2574	rBV	234	93	0.01%	0.002%
46	9.326	2574	2577	2580	rVV3	271	202	0.03%	0.004%
47	9.648	2676	2677	2678	rBV	162	49	0.01%	0.001%
48	10.050	2800	2802	2805	rBV	180	124	0.02%	0.002%
49	10.130	2822	2827	2828	rBV3	1165	1133	0.17%	0.020%
50	10.217	2843	2854	2868	rBV	182161	288782	43.79%	5.208%
51	10.320	2884	2886	2888	rBV2	320	130	0.02%	0.002%
52	10.686	2996	3000	3002	rBV	241	170	0.03%	0.003%
53	10.911	3065	3070	3074	rBV4	1170	1286	0.20%	0.023%
54	11.249	3164	3175	3194	rBV	374418	578377	87.71%	10.430%
55	11.625	3280	3292	3313	rBV	301567	474454	71.95%	8.556%
56	11.786	3338	3342	3346	rBV2	812	616	0.09%	0.011%
57	11.873	3367	3369	3371	rBV2	366	192	0.03%	0.003%
58	12.111	3441	3443	3448	rVB2	489	344	0.05%	0.006%
59	13.632	3914	3916	3920	rBV	513	363	0.06%	0.007%
60	13.988	4025	4027	4029	rBV	343	124	0.02%	0.002%
61	14.072	4051	4053	4058	rVB2	374	187	0.03%	0.003%
62	14.763	4266	4268	4271	rBV2	472	296	0.04%	0.005%
63	15.275	4425	4427	4429	rBV	367	223	0.03%	0.004%




Sum of corrected areas: 5545462

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101221\
Data File : VV022753.D
Acq On : 12 Oct 2021 14:58
Operator : SY/MD
Sample : M4125-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGB16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

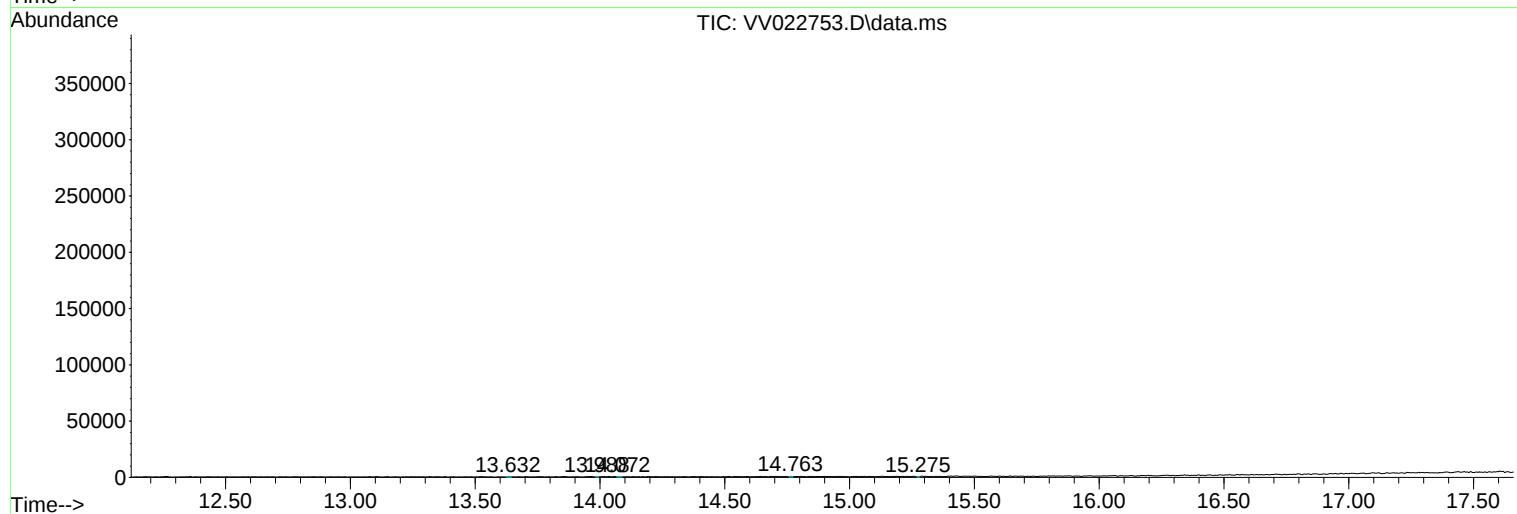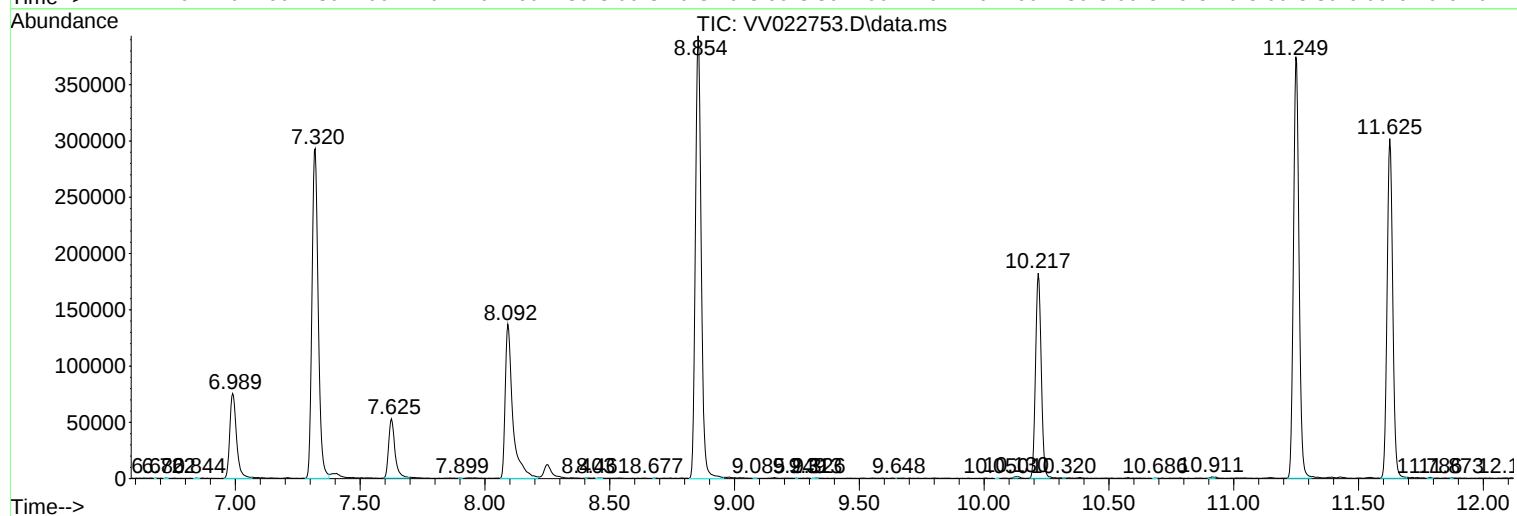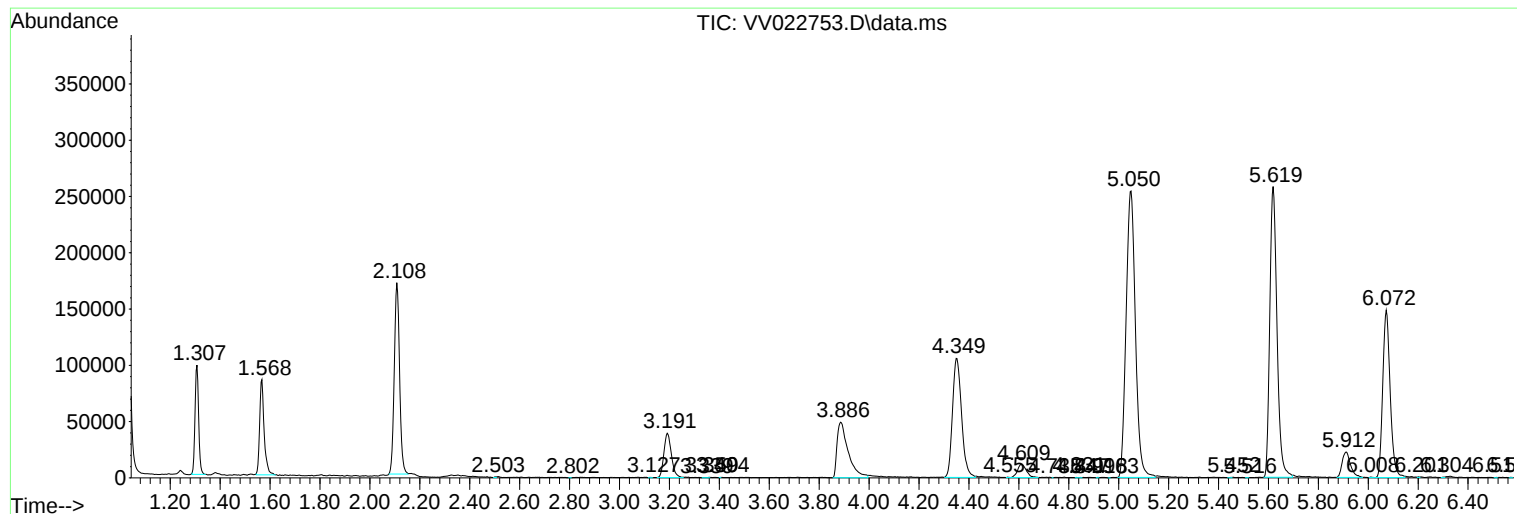

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101221\
Data File : VV022753.D
Acq On : 12 Oct 2021 14:58
Operator : SY/MD
Sample : M4125-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGB16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101221\
Data File : VV022753.D
Acq On : 12 Oct 2021 14:58
Operator : SY/MD
Sample : M4125-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGB16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
