
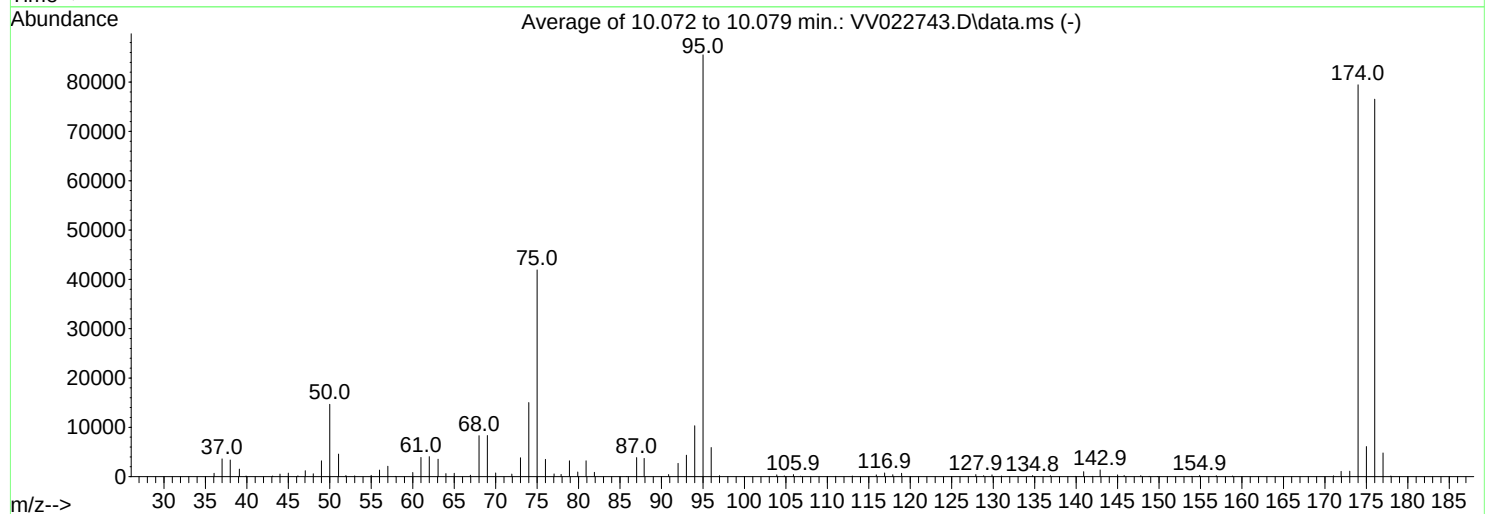


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101221\
 Data File : VV022743.D
 Acq On : 12 Oct 2021 09:11
 Operator : SY/MD
 Sample : BFB241
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB241

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis
 Last Update : Wed Oct 13 01:15:35 2021

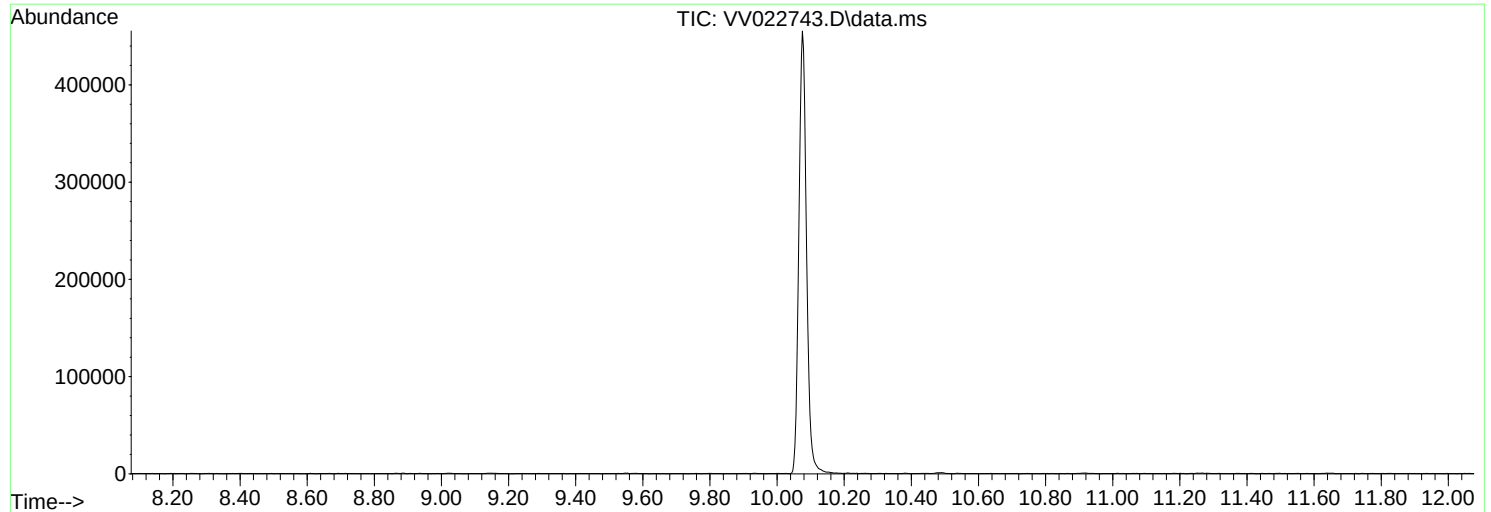

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	14670	PASS
75	95	30	80	49.0	41923	PASS
95	95	100	100	100.0	85523	PASS
96	95	5	9	6.9	5896	PASS
173	174	0.00	2	1.4	1117	PASS
174	95	50	120	92.9	79448	PASS
175	174	5	9	7.7	6095	PASS
176	174	95	105	96.3	76544	PASS
177	176	5	10	6.3	4819	PASS

Scan 2798 (10.037 min): VV022743.D\data.ms
BFB241

m/z	Abundance
39.90	107.0
43.90	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

m/z	Abundance
36.10	617.0
37.00	3807.0
38.00	3332.0
39.10	1530.0
39.90	228.0
43.10	114.0
44.10	686.0
45.00	719.0
46.20	147.0
47.00	1098.0
48.00	547.0
49.00	3318.0
50.00	14457.0
51.10	4473.0
52.00	290.0
53.00	152.0
55.00	281.0
56.00	1295.0
57.00	2096.0
60.00	881.0
61.00	3959.0
62.00	3977.0
63.00	3478.0
64.00	629.0
65.00	694.0
66.90	271.0
68.00	8538.0
69.00	8185.0
70.00	756.0
72.00	477.0
73.00	3690.0
74.00	14652.0
75.00	40976.0
76.00	3481.0
77.00	538.0
77.90	451.0
78.90	3176.0
79.90	911.0
80.90	3244.0
81.90	874.0
85.80	118.0
87.00	3660.0
87.90	3581.0
90.80	354.0
92.00	2582.0
93.00	4304.0
94.00	10074.0
95.00	84072.0
96.00	5802.0
97.00	197.0
103.90	365.0
104.80	126.0
105.90	425.0
106.80	104.0
111.00	130.0
113.00	137.0
115.80	375.0
116.90	716.0
117.90	438.0
119.00	611.0
127.90	428.0
128.80	223.0
129.90	343.0
130.90	147.0
134.70	193.0
136.90	166.0
140.90	945.0
141.90	108.0
142.90	1341.0
145.00	327.0
145.80	217.0
147.80	179.0
149.80	115.0
154.90	235.0
156.90	216.0
159.00	145.0
171.10	153.0
171.90	1079.0
173.00	1158.0
174.00	75752.0
175.00	6046.0
176.00	72952.0
177.00	4704.0
178.00	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

m/z	Abundance
36.10	696.0
37.00	3694.0
38.00	3458.0
39.10	1577.0
40.00	226.0
43.10	124.0
44.00	661.0
45.00	767.0
46.20	173.0
47.10	1265.0
48.00	627.0
49.00	3281.0
50.00	15315.0
51.00	4723.0
52.00	227.0
53.00	186.0
55.00	277.0
56.00	1360.0
57.00	2183.0
57.90	102.0
60.00	905.0
61.00	4028.0
62.00	4168.0
63.00	3648.0
64.00	643.0
65.00	707.0
67.00	291.0
68.00	8632.0
69.00	8590.0
70.00	797.0
71.90	536.0
73.00	3940.0
74.00	15577.0
75.00	43328.0
76.00	3647.0
77.10	564.0
77.90	463.0
78.90	3351.0
79.90	966.0
80.90	3341.0
81.90	908.0
87.00	3996.0
87.90	3795.0
90.90	424.0
92.00	2797.0
93.00	4515.0
94.00	10627.0
95.00	88240.0
96.00	6165.0
97.00	187.0
103.90	349.0
104.80	159.0
105.90	461.0
106.80	108.0
111.00	101.0
113.00	157.0
115.90	387.0
116.90	764.0
117.90	422.0
119.00	707.0
127.90	465.0
128.80	207.0
129.80	357.0
131.00	144.0
134.70	230.0
136.90	199.0
139.90	103.0
140.90	1051.0
142.00	112.0
142.90	1411.0
145.00	354.0
145.80	254.0
147.80	207.0
148.80	116.0
153.90	119.0
154.90	283.0
156.90	217.0
158.80	113.0
171.00	194.0
171.90	1132.0
173.00	1153.0
174.00	82312.0
175.00	6256.0
176.00	79016.0
177.00	4937.0
177.90	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

m/z	Abundance
36.00	710.0
37.00	3331.0
38.00	3304.0
39.10	1476.0
40.00	215.0
43.10	131.0
44.00	579.0
45.00	697.0
46.10	157.0
47.10	1232.0
48.00	632.0
49.00	3031.0
50.00	14238.0
51.00	4555.0
51.90	175.0
53.00	190.0
55.00	241.0
56.00	1297.0
57.00	2071.0
57.90	118.0
60.00	804.0
61.00	3709.0
62.00	4074.0
63.10	3461.0
64.00	582.0
65.00	696.0
67.00	278.0
68.00	7787.0
69.00	8268.0
70.00	718.0
72.00	549.0
73.00	3868.0
74.00	14878.0
75.00	41464.0
76.00	3401.0
77.10	524.0
77.90	436.0
78.90	3120.0
79.90	931.0
80.90	3043.0
81.90	817.0
87.00	3933.0
87.90	3684.0
90.90	449.0
92.00	2683.0
93.00	4189.0
94.00	10214.0
95.00	84256.0
96.00	5720.0
97.00	158.0
103.90	332.0
104.80	168.0
105.90	428.0
106.80	122.0
110.00	109.0
113.00	142.0
116.00	364.0
116.90	749.0
117.90	356.0
118.90	710.0
127.90	394.0
128.90	171.0
129.80	366.0
131.10	135.0
134.80	213.0
136.90	203.0
139.90	121.0
140.90	994.0
142.90	1321.0
145.00	362.0
145.80	247.0
147.80	199.0
148.80	102.0
153.90	117.0
154.90	272.0
156.90	176.0
158.70	117.0
171.00	191.0
172.00	1048.0
173.00	1039.0
174.00	80280.0
175.00	5982.0
176.00	77664.0
177.00	4816.0
177.90	147.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241