

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101222\
 Data File : VV028526.D
 Acq On : 12 Oct 2022 12:27
 Operator : SY/MD
 Sample : VV1012MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK279

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	187906	199102	12.81%	1.783%
2	1.564	157	163	176	rVB	145532	165103	10.62%	1.478%
3	2.101	322	330	346	rVB	300765	430508	27.70%	3.854%
4	2.568	473	475	477	rBV2	588	312	0.02%	0.003%
5	2.654	500	502	506	rBV3	628	562	0.04%	0.005%
6	2.715	518	521	525	rBV3	465	376	0.02%	0.003%
7	2.735	525	527	529	rVB3	640	278	0.02%	0.002%
8	2.748	529	531	533	rBV	991	556	0.04%	0.005%
9	2.760	533	535	538	rVV3	811	475	0.03%	0.004%
10	2.777	538	540	543	rVB	676	275	0.02%	0.002%
11	2.918	578	584	589	rVV4	864	843	0.05%	0.008%
12	3.005	608	611	614	rBV3	674	553	0.04%	0.005%
13	3.021	614	616	618	rVV2	656	348	0.02%	0.003%
14	3.043	621	623	626	rVB4	662	363	0.02%	0.003%
15	3.114	642	645	650	rBV4	563	569	0.04%	0.005%
16	3.195	667	670	674	rVB2	434	295	0.02%	0.003%
17	3.217	674	677	679	rBV3	317	220	0.01%	0.002%
18	3.252	685	688	693	rBV3	617	469	0.03%	0.004%
19	3.516	765	770	772	rBV2	544	500	0.03%	0.004%
20	3.629	799	805	808	rVB3	560	468	0.03%	0.004%
21	3.693	822	825	827	rBV3	611	392	0.03%	0.004%
22	3.892	875	887	921	rBV	76899	305454	19.66%	2.735%
23	4.339	1013	1026	1063	rVB	242516	607347	39.08%	5.438%
24	4.664	1124	1127	1128	rBV2	557	247	0.02%	0.002%
25	4.741	1149	1151	1157	rVB2	656	424	0.03%	0.004%
26	4.860	1185	1188	1191	rBV2	379	242	0.02%	0.002%
27	4.899	1197	1200	1204	rVB4	851	549	0.04%	0.005%
28	4.934	1208	1211	1215	rBV2	568	422	0.03%	0.004%
29	5.037	1226	1243	1273	rBV2	596179	1554046	100.00%	13.913%
30	5.339	1335	1337	1341	rBV4	613	536	0.03%	0.005%
31	5.381	1347	1350	1351	rBV3	499	236	0.02%	0.002%
32	5.474	1376	1379	1380	rBV	393	219	0.01%	0.002%
33	5.513	1389	1391	1395	rBV3	351	323	0.02%	0.003%
34	5.555	1401	1404	1405	rBV	393	225	0.01%	0.002%
35	5.609	1410	1421	1457	rBV	390741	801491	51.57%	7.176%
36	5.908	1503	1514	1518	rBV5	3992	7033	0.45%	0.063%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101222\
 Data File : VV028526.D
 Acq On : 12 Oct 2022 12:27
 Operator : SY/MD
 Sample : VV1012MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK279

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.063	1548	1562	1592	rBV	340060	702547	45.21%	6.290%
38	6.426	1670	1675	1676	rBV	405	282	0.02%	0.003%
39	6.632	1737	1739	1743	rVB2	349	227	0.01%	0.002%
40	6.702	1758	1761	1764	rVV4	375	244	0.02%	0.002%
41	6.818	1793	1797	1801	rBV2	564	345	0.02%	0.003%
42	6.860	1806	1810	1814	rVB2	525	308	0.02%	0.003%
43	6.886	1814	1818	1822	rBV3	500	411	0.03%	0.004%
44	6.979	1835	1847	1877	rBV	210649	394820	25.41%	3.535%
45	7.198	1912	1915	1918	rBV3	920	670	0.04%	0.006%
46	7.310	1938	1950	1983	rBV	688966	1239672	79.77%	11.099%
47	7.561	2027	2028	2032	rVB3	578	301	0.02%	0.003%
48	7.616	2035	2045	2068	rBV	143134	259508	16.70%	2.323%
49	7.837	2111	2114	2118	rVB2	593	382	0.02%	0.003%
50	7.860	2118	2121	2124	rVB2	602	324	0.02%	0.003%
51	7.889	2128	2130	2137	rVB3	465	349	0.02%	0.003%
52	7.924	2137	2141	2142	rBV	447	261	0.02%	0.002%
53	7.953	2148	2150	2153	rBV3	405	264	0.02%	0.002%
54	8.046	2174	2179	2180	rBV3	513	446	0.03%	0.004%
55	8.085	2181	2191	2229	rBV	367790	779789	50.18%	6.982%
56	8.844	2416	2427	2450	rBV	570298	942917	60.67%	8.442%
57	9.149	2517	2522	2524	rBV3	793	615	0.04%	0.006%
58	9.197	2534	2537	2538	rBV2	308	217	0.01%	0.002%
59	9.223	2543	2545	2548	rVB3	691	335	0.02%	0.003%
60	9.265	2552	2558	2560	rBV3	350	335	0.02%	0.003%
61	9.304	2566	2570	2572	rBV2	287	234	0.02%	0.002%
62	9.429	2606	2609	2615	rVB2	458	379	0.02%	0.003%
63	9.474	2621	2623	2627	rVB3	492	312	0.02%	0.003%
64	9.535	2639	2642	2643	rBV	714	341	0.02%	0.003%
65	9.590	2657	2659	2662	rVB2	756	369	0.02%	0.003%
66	9.744	2705	2707	2712	rVB2	432	297	0.02%	0.003%
67	9.789	2716	2721	2722	rBV3	446	334	0.02%	0.003%
68	9.914	2755	2760	2761	rBV2	663	433	0.03%	0.004%
69	10.082	2807	2812	2816	rBV4	681	536	0.03%	0.005%
70	10.111	2816	2821	2822	rBV3	328	237	0.02%	0.002%
71	10.207	2839	2851	2872	rBV	428611	685238	44.09%	6.135%
72	10.432	2920	2921	2926	rVV2	445	312	0.02%	0.003%
73	10.535	2950	2953	2959	rVB3	770	650	0.04%	0.006%
74	10.593	2969	2971	2973	rBV	458	220	0.01%	0.002%
75	10.699	3002	3004	3007	rBV	555	339	0.02%	0.003%
76	10.734	3013	3015	3019	rBV2	320	244	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101222\
 Data File : VV028526.D
 Acq On : 12 Oct 2022 12:27
 Operator : SY/MD
 Sample : VV1012MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK279

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	10.773	3025	3027	3030	rVB	506	297	0.02%	0.003%
78	10.863	3053	3055	3058	rBV3	552	350	0.02%	0.003%
79	10.995	3092	3096	3101	rBV2	330	309	0.02%	0.003%
80	11.059	3114	3116	3118	rVB2	587	250	0.02%	0.002%
81	11.075	3118	3121	3124	rVB	389	301	0.02%	0.003%
82	11.107	3127	3131	3136	rBV3	436	445	0.03%	0.004%
83	11.181	3149	3154	3161	rBV6	1425	2201	0.14%	0.020%
84	11.239	3161	3172	3195	rBV	619689	971071	62.49%	8.694%
85	11.477	3244	3246	3250	rBV2	336	227	0.01%	0.002%
86	11.558	3267	3271	3273	rBV2	549	294	0.02%	0.003%
87	11.615	3277	3289	3311	rVV	684208	1085301	69.84%	9.717%
88	12.149	3450	3455	3457	rBV	364	326	0.02%	0.003%
89	12.184	3464	3466	3471	rBV2	438	340	0.02%	0.003%
90	12.451	3547	3549	3551	rVB2	468	228	0.01%	0.002%
91	12.464	3551	3553	3558	rVB2	401	303	0.02%	0.003%
92	12.673	3616	3618	3624	rVB2	352	214	0.01%	0.002%
93	12.892	3684	3686	3688	rBV3	432	226	0.01%	0.002%
94	13.213	3783	3786	3788	rBV2	382	312	0.02%	0.003%
95	13.265	3795	3802	3808	rVB5	2304	2590	0.17%	0.023%
96	13.339	3822	3825	3827	rBV2	492	307	0.02%	0.003%
97	13.352	3827	3829	3831	rBV2	459	238	0.02%	0.002%
98	13.689	3932	3934	3935	rBV	570	251	0.02%	0.002%
99	13.747	3941	3952	3955	rBV7	3264	5257	0.34%	0.047%
100	14.194	4089	4091	4094	rBV2	402	315	0.02%	0.003%




Sum of corrected areas: 11169358

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101222\
Data File : VV028526.D
Acq On : 12 Oct 2022 12:27
Operator : SY/MD
Sample : VV1012MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK279

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

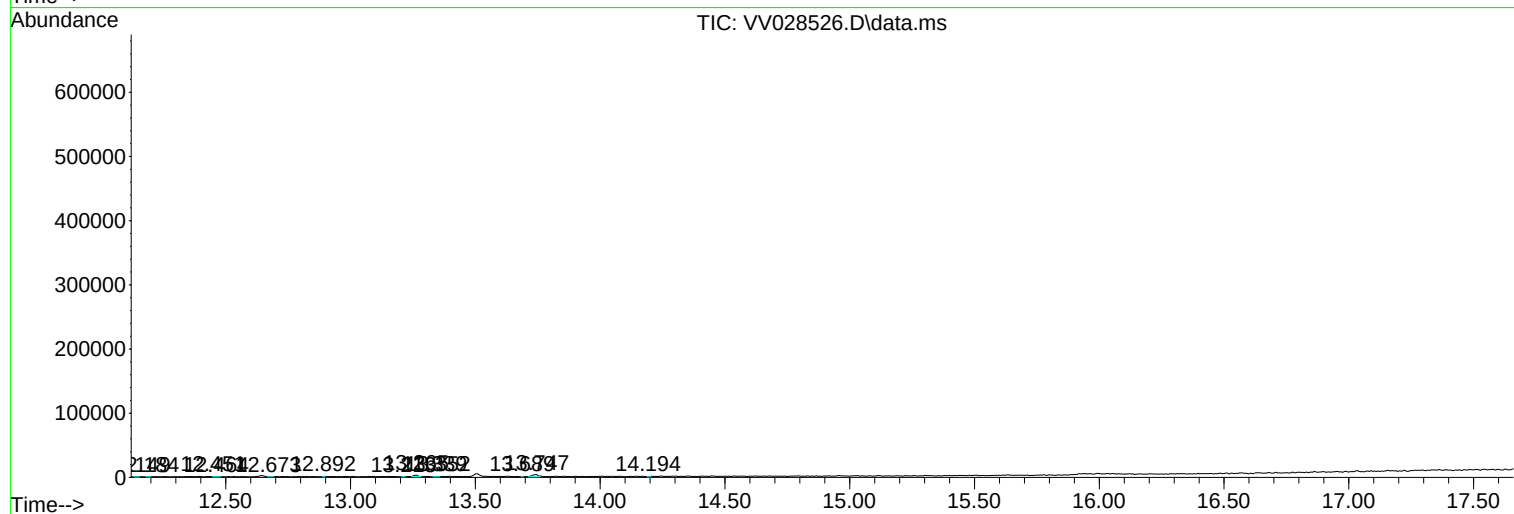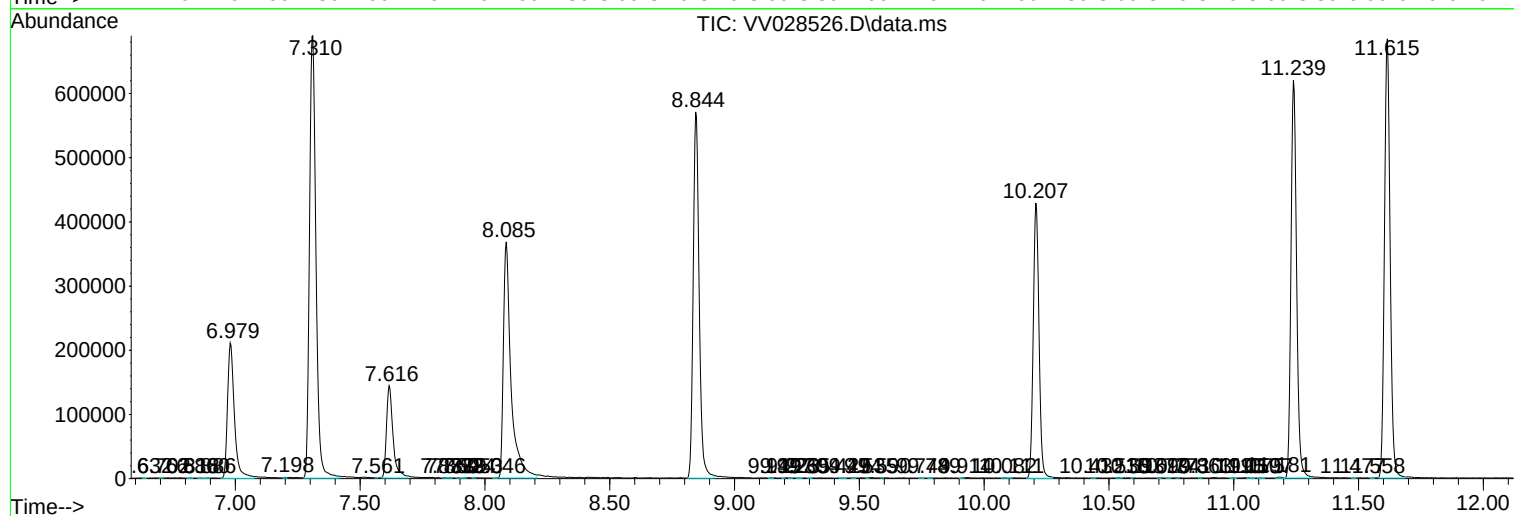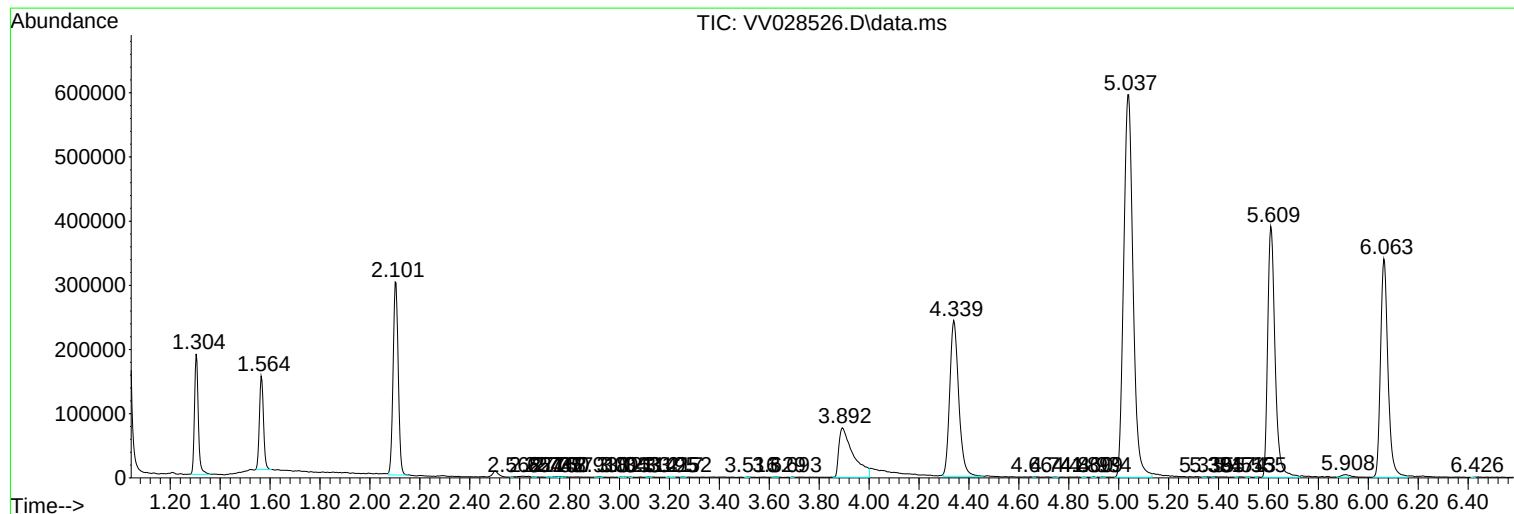

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101222\
Data File : VV028526.D
Acq On : 12 Oct 2022 12:27
Operator : SY/MD
Sample : VV1012MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK279

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101222\
Data File : VV028526.D
Acq On : 12 Oct 2022 12:27
Operator : SY/MD
Sample : VV1012MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK279

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc