

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101222\
 Data File : VV028527.D
 Acq On : 12 Oct 2022 12:51
 Operator : SY/MD
 Sample : VV1012WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK280

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	175374	181282	12.02%	1.689%
2	1.568	157	164	178	rVB	142971	161123	10.68%	1.501%
3	2.105	322	331	349	rVB	285947	417794	27.69%	3.892%
4	2.507	447	456	469	rVB2	9017	16628	1.10%	0.155%
5	2.738	524	528	530	rBV2	597	459	0.03%	0.004%
6	2.809	546	550	554	rBV2	494	376	0.02%	0.004%
7	2.902	574	579	580	rBV	555	355	0.02%	0.003%
8	2.986	603	605	607	rVV	546	190	0.01%	0.002%
9	3.031	617	619	622	rVB2	413	209	0.01%	0.002%
10	3.101	638	641	643	rBV3	323	197	0.01%	0.002%
11	3.117	643	646	648	rVB	456	251	0.02%	0.002%
12	3.130	648	650	652	rBV2	408	208	0.01%	0.002%
13	3.230	679	681	685	rBV2	369	349	0.02%	0.003%
14	3.272	691	694	697	rBV2	444	309	0.02%	0.003%
15	3.391	727	731	733	rBV2	387	335	0.02%	0.003%
16	3.420	738	740	741	rBV	454	233	0.02%	0.002%
17	3.510	766	768	770	rBV2	334	215	0.01%	0.002%
18	3.542	776	778	783	rBV3	482	369	0.02%	0.003%
19	3.584	789	791	795	rBV3	490	273	0.02%	0.003%
20	3.690	821	824	827	rVB	555	330	0.02%	0.003%
21	3.722	832	834	836	rBV3	578	212	0.01%	0.002%
22	3.818	857	864	871	rBV4	611	812	0.05%	0.008%
23	3.899	874	889	920	rBV	71459	296133	19.63%	2.759%
24	4.342	1014	1027	1057	rVB	227366	570869	37.84%	5.318%
25	4.648	1120	1122	1125	rBV3	498	204	0.01%	0.002%
26	4.683	1131	1133	1135	rBV2	615	341	0.02%	0.003%
27	4.744	1148	1152	1157	rVB2	500	469	0.03%	0.004%
28	4.796	1166	1168	1169	rBV2	450	201	0.01%	0.002%
29	4.915	1200	1205	1208	rBV3	617	536	0.04%	0.005%
30	4.941	1208	1213	1216	rBV5	573	628	0.04%	0.006%
31	5.040	1227	1244	1286	rBV2	577169	1508783	100.00%	14.055%
32	5.404	1354	1357	1360	rVB5	1190	792	0.05%	0.007%
33	5.420	1360	1362	1365	rBV3	770	551	0.04%	0.005%
34	5.477	1376	1380	1384	rBV4	866	724	0.05%	0.007%
35	5.500	1384	1387	1390	rBV3	371	288	0.02%	0.003%
36	5.535	1396	1398	1400	rVB	553	192	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101222\
 Data File : VV028527.D
 Acq On : 12 Oct 2022 12:51
 Operator : SY/MD
 Sample : VV1012WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK280

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	5.613	1407	1422	1450	rBV	377882	770335	51.06%	7.176%
38	5.799	1476	1480	1483	rBV5	1057	947	0.06%	0.009%
39	6.066	1549	1563	1588	rBV	329529	678204	44.95%	6.318%
40	6.339	1647	1648	1652	rVB	476	272	0.02%	0.003%
41	6.362	1652	1655	1657	rBV2	396	244	0.02%	0.002%
42	6.706	1759	1762	1765	rVB2	854	605	0.04%	0.006%
43	6.741	1771	1773	1776	rVB2	399	234	0.02%	0.002%
44	6.783	1784	1786	1790	rVB2	291	195	0.01%	0.002%
45	6.812	1790	1795	1798	rBV2	312	255	0.02%	0.002%
46	6.834	1800	1802	1807	rVB2	413	259	0.02%	0.002%
47	6.892	1818	1820	1823	rBV2	371	213	0.01%	0.002%
48	6.908	1823	1825	1827	rBV2	449	227	0.02%	0.002%
49	6.982	1832	1848	1874	rBV	203182	380789	25.24%	3.547%
50	7.310	1939	1950	1972	rBV	673588	1172352	77.70%	10.921%
51	7.616	2036	2045	2072	rBV	136473	249651	16.55%	2.326%
52	7.879	2125	2127	2135	rVB5	882	867	0.06%	0.008%
53	7.918	2137	2139	2142	rVB	740	345	0.02%	0.003%
54	7.937	2142	2145	2146	rBV	882	461	0.03%	0.004%
55	7.963	2151	2153	2156	rBV2	604	332	0.02%	0.003%
56	8.085	2180	2191	2224	rBV	364842	779675	51.68%	7.263%
57	8.606	2349	2353	2354	rBV3	423	320	0.02%	0.003%
58	8.664	2368	2371	2373	rBV2	394	271	0.02%	0.003%
59	8.677	2373	2375	2380	rVB4	731	426	0.03%	0.004%
60	8.719	2386	2388	2391	rBV3	550	354	0.02%	0.003%
61	8.735	2391	2393	2397	rVB3	474	301	0.02%	0.003%
62	8.792	2407	2411	2415	rVB3	463	323	0.02%	0.003%
63	8.847	2415	2428	2459	rBV	536397	905475	60.01%	8.435%
64	9.098	2503	2506	2510	rBV3	507	400	0.03%	0.004%
65	9.114	2510	2511	2514	rVV2	516	281	0.02%	0.003%
66	9.143	2517	2520	2528	rVB4	1058	1162	0.08%	0.011%
67	9.297	2566	2568	2571	rBV2	344	230	0.02%	0.002%
68	9.349	2578	2584	2588	rVB4	359	438	0.03%	0.004%
69	9.403	2599	2601	2603	rVB2	517	256	0.02%	0.002%
70	9.432	2603	2610	2612	rBV2	427	378	0.03%	0.004%
71	9.529	2636	2640	2643	rBV3	559	476	0.03%	0.004%
72	9.590	2655	2659	2661	rVB2	609	347	0.02%	0.003%
73	9.648	2675	2677	2682	rVB2	278	204	0.01%	0.002%
74	9.854	2737	2741	2743	rBV2	324	269	0.02%	0.003%
75	9.982	2779	2781	2783	rVB2	517	201	0.01%	0.002%
76	10.066	2804	2807	2810	rBV2	413	311	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101222\
 Data File : VV028527.D
 Acq On : 12 Oct 2022 12:51
 Operator : SY/MD
 Sample : VV1012WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK280

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	10.143	2828	2831	2834	rVB2	555	285	0.02%	0.003%
78	10.207	2839	2851	2878	rBV	427381	676474	44.84%	6.302%
79	10.355	2894	2897	2900	rVB2	591	378	0.03%	0.004%
80	10.374	2901	2903	2905	rVB2	551	247	0.02%	0.002%
81	10.596	2969	2972	2975	rBV	427	294	0.02%	0.003%
82	10.657	2987	2991	2992	rBV3	405	247	0.02%	0.002%
83	10.786	3026	3031	3033	rBV2	487	419	0.03%	0.004%
84	10.850	3049	3051	3057	rVB3	491	301	0.02%	0.003%
85	10.918	3069	3072	3078	rVB3	822	597	0.04%	0.006%
86	11.111	3129	3132	3134	rBV2	465	242	0.02%	0.002%
87	11.172	3148	3151	3152	rBV3	520	251	0.02%	0.002%
88	11.239	3161	3172	3198	rBV	572010	912907	60.51%	8.504%
89	11.374	3212	3214	3217	rBV2	405	212	0.01%	0.002%
90	11.616	3277	3289	3311	rBV	640241	1026211	68.02%	9.560%
91	11.841	3357	3359	3361	rBV2	409	224	0.01%	0.002%
92	11.863	3363	3366	3369	rBV	282	232	0.02%	0.002%
93	12.008	3408	3411	3414	rVB2	525	355	0.02%	0.003%
94	12.037	3415	3420	3424	rBV2	442	514	0.03%	0.005%
95	12.204	3467	3472	3477	rBV3	551	519	0.03%	0.005%
96	12.416	3534	3538	3541	rBV3	478	444	0.03%	0.004%
97	12.895	3684	3687	3689	rBV2	441	333	0.02%	0.003%
98	13.046	3732	3734	3736	rBV	433	247	0.02%	0.002%
99	13.297	3809	3812	3814	rBV2	663	481	0.03%	0.004%
100	13.972	4019	4022	4025	rVB3	738	418	0.03%	0.004%


Sum of corrected areas: 10734937

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101222\
Data File : VV028527.D
Acq On : 12 Oct 2022 12:51
Operator : SY/MD
Sample : VV1012WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK280

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

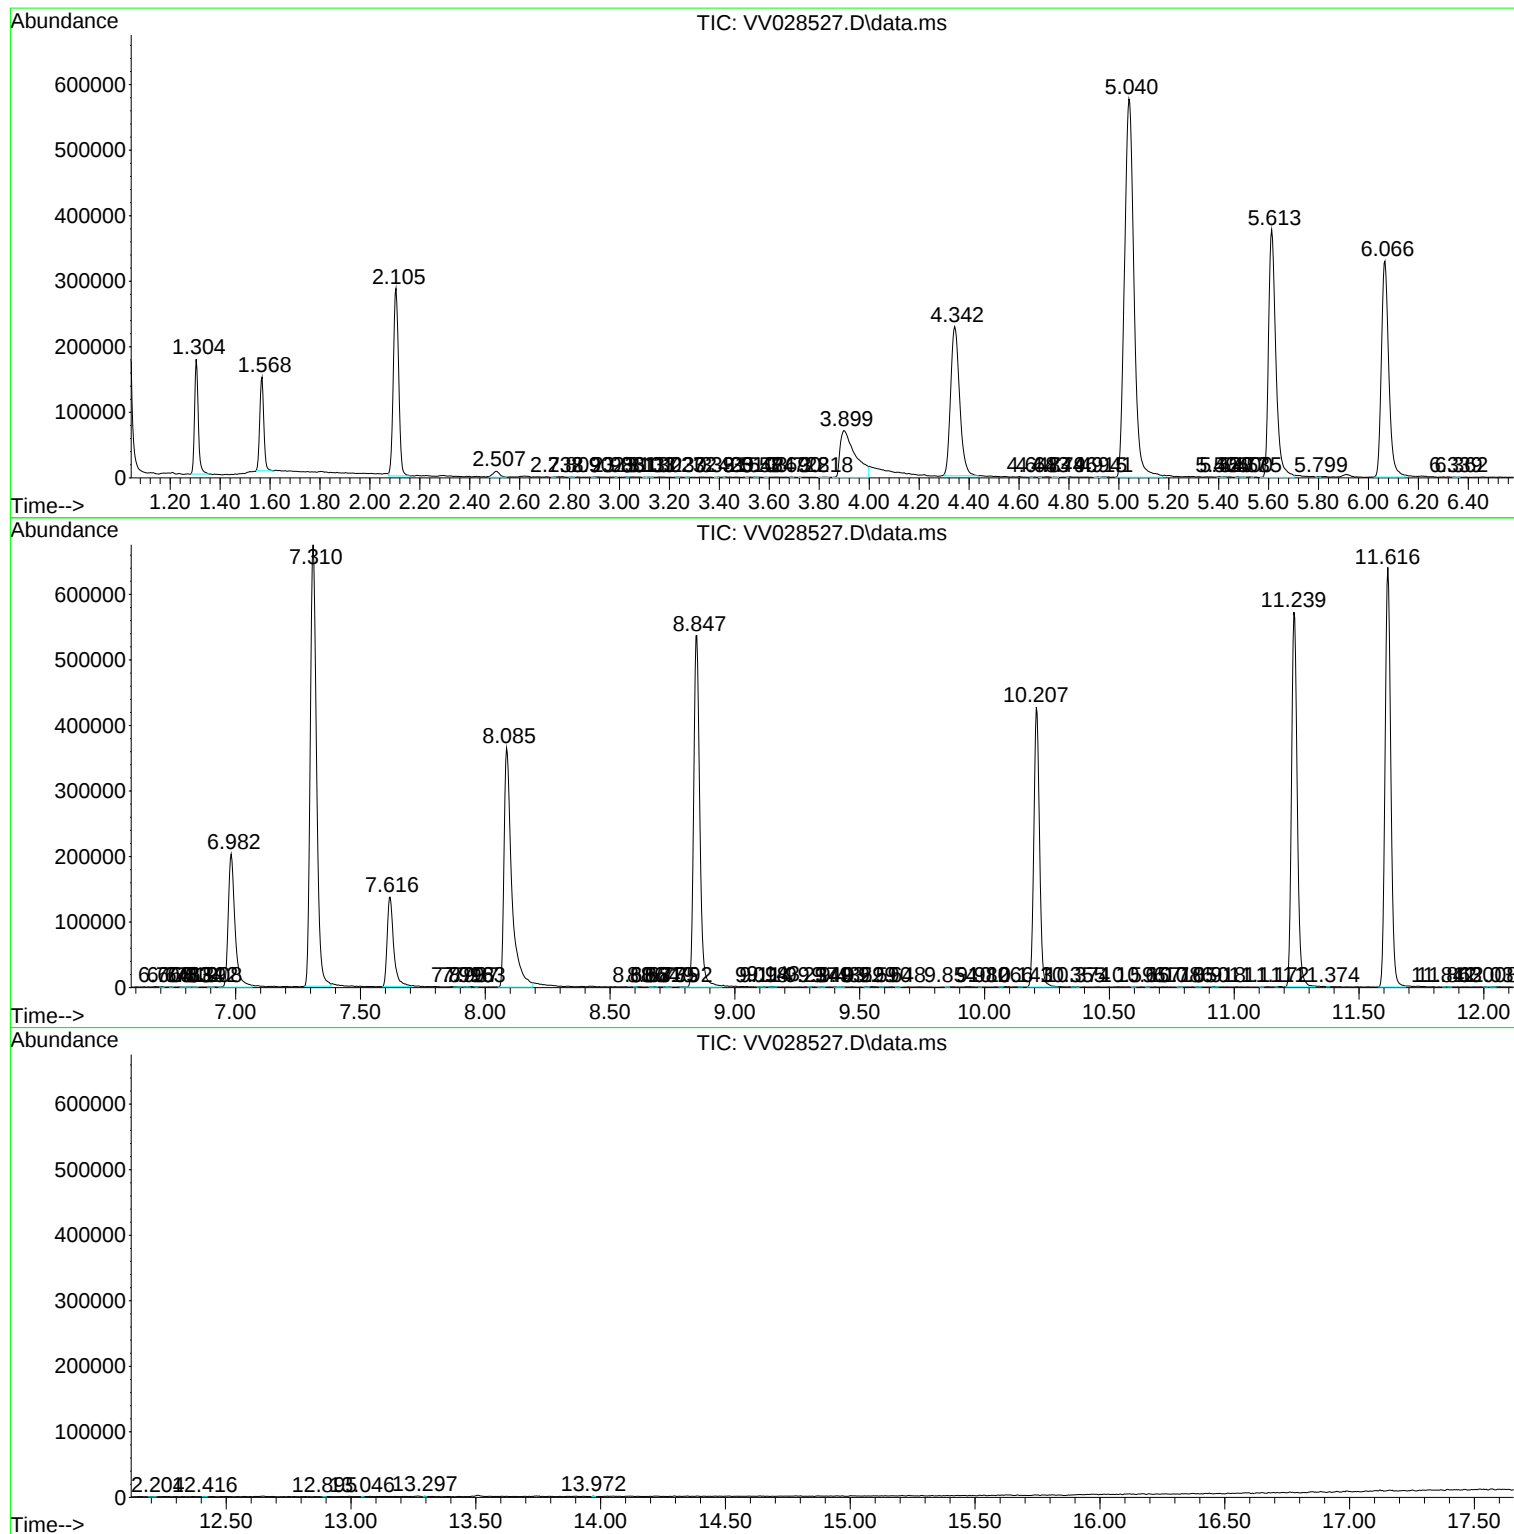

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101222\
Data File : VV028527.D
Acq On : 12 Oct 2022 12:51
Operator : SY/MD
Sample : VV1012WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK280

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101222\
Data File : VV028527.D
Acq On : 12 Oct 2022 12:51
Operator : SY/MD
Sample : VV1012WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK280

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------