

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101222\
 Data File : VV028532.D
 Acq On : 12 Oct 2022 17:12
 Operator : SY/MD
 Sample : N5064-17ME
 Misc : 7.52g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BN6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028532.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	104	rBV	116418	154565	8.65%	1.087%
2	1.564	157	163	186	rBV	102211	157450	8.81%	1.108%
3	2.092	319	327	344	rVB	373293	528210	29.57%	3.716%
4	2.834	557	558	560	rBV	275	121	0.01%	0.001%
5	2.851	561	563	565	rVB	387	167	0.01%	0.001%
6	2.883	570	573	575	rBV2	344	239	0.01%	0.002%
7	3.098	637	640	642	rBV	252	181	0.01%	0.001%
8	3.252	682	688	691	rBV2	329	294	0.02%	0.002%
9	3.272	692	694	698	rVB	232	128	0.01%	0.001%
10	3.320	706	709	714	rVB2	297	226	0.01%	0.002%
11	3.343	714	716	719	rBV	234	140	0.01%	0.001%
12	3.535	773	776	779	rVB2	336	167	0.01%	0.001%
13	3.561	781	784	787	rBV2	159	136	0.01%	0.001%
14	3.616	798	801	802	rBV2	272	156	0.01%	0.001%
15	3.674	816	819	823	rVB2	344	240	0.01%	0.002%
16	3.725	825	835	838	rBV2	291	419	0.02%	0.003%
17	3.902	878	890	945	rBV	63696	382298	21.40%	2.689%
18	4.336	1013	1025	1055	rVB	304897	758995	42.49%	5.340%
19	4.735	1147	1149	1151	rBV	248	132	0.01%	0.001%
20	4.818	1172	1175	1176	rBV	332	184	0.01%	0.001%
21	4.867	1185	1190	1193	rBV	220	240	0.01%	0.002%
22	4.902	1198	1201	1206	rBV2	288	323	0.02%	0.002%
23	5.037	1225	1243	1276	rBV2	690424	1786456	100.00%	12.568%
24	5.609	1408	1421	1457	rBV	511654	1035859	57.98%	7.287%
25	5.905	1504	1513	1522	rBV8	6048	12227	0.68%	0.086%
26	6.063	1549	1562	1595	rBV	402667	846047	47.36%	5.952%
27	6.291	1630	1633	1635	rBV2	515	299	0.02%	0.002%
28	6.304	1635	1637	1639	rVB	385	131	0.01%	0.001%
29	6.365	1653	1656	1658	rBV	447	262	0.01%	0.002%
30	6.436	1676	1678	1682	rVB2	223	144	0.01%	0.001%
31	6.535	1706	1709	1714	rBV2	293	232	0.01%	0.002%
32	6.638	1731	1741	1743	rBV4	2873	3398	0.19%	0.024%
33	6.911	1824	1826	1829	rVB2	433	239	0.01%	0.002%
34	6.931	1829	1832	1836	rVB	265	153	0.01%	0.001%
35	6.979	1836	1847	1877	rBV	257533	489415	27.40%	3.443%
36	7.310	1937	1950	1979	rBV	793283	1401199	78.43%	9.858%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101222\
 Data File : VW028532.D
 Acq On : 12 Oct 2022 17:12
 Operator : SY/MD
 Sample : N5064-17ME
 Misc : 7.52g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBN6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	7.571	2028	2031	2033	rBV3	414	208	0.01%	0.001%
38	7.616	2035	2045	2086	rVV	176086	341322	19.11%	2.401%
39	7.876	2124	2126	2128	rBV	410	171	0.01%	0.001%
40	7.969	2153	2155	2157	rBV2	424	210	0.01%	0.001%
41	8.101	2183	2196	2236	rBV	388690	1094402	61.26%	7.699%
42	8.432	2290	2299	2311	rVB4	3397	5957	0.33%	0.042%
43	8.535	2329	2331	2337	rVB3	462	350	0.02%	0.002%
44	8.567	2337	2341	2343	rBV3	291	223	0.01%	0.002%
45	8.657	2365	2369	2373	rBV2	340	329	0.02%	0.002%
46	8.847	2415	2428	2456	rBV	719792	1242784	69.57%	8.743%
47	9.059	2491	2494	2497	rVB	987	543	0.03%	0.004%
48	9.075	2497	2499	2502	rBV2	364	234	0.01%	0.002%
49	9.133	2514	2517	2518	rBV2	449	258	0.01%	0.002%
50	9.198	2535	2537	2539	rVB	367	144	0.01%	0.001%
51	9.223	2542	2545	2547	rBV2	228	138	0.01%	0.001%
52	9.278	2558	2562	2564	rBV2	209	148	0.01%	0.001%
53	9.326	2574	2577	2579	rBV	451	151	0.01%	0.001%
54	9.397	2595	2599	2603	rBV2	279	211	0.01%	0.001%
55	9.693	2688	2691	2693	rBV2	279	135	0.01%	0.001%
56	9.786	2716	2720	2727	rVB2	383	268	0.02%	0.002%
57	9.831	2727	2734	2735	rBV2	230	209	0.01%	0.001%
58	9.879	2744	2749	2753	rVB	256	272	0.02%	0.002%
59	9.905	2753	2757	2761	rBV2	134	127	0.01%	0.001%
60	9.934	2761	2766	2768	rBV3	622	547	0.03%	0.004%
61	10.014	2789	2791	2795	rVB2	228	152	0.01%	0.001%
62	10.082	2809	2812	2815	rBV2	276	158	0.01%	0.001%
63	10.214	2837	2853	2875	rBV	598680	993126	55.59%	6.987%
64	10.362	2897	2899	2901	rBV2	423	269	0.02%	0.002%
65	10.439	2921	2923	2926	rBV2	295	149	0.01%	0.001%
66	10.522	2945	2949	2950	rBV	230	137	0.01%	0.001%
67	10.577	2959	2966	2974	rVB7	2917	4049	0.23%	0.028%
68	10.609	2974	2976	2980	rVB2	231	142	0.01%	0.001%
69	10.628	2980	2982	2986	rVB	280	161	0.01%	0.001%
70	10.657	2986	2991	2996	rVB2	267	202	0.01%	0.001%
71	10.686	2996	3000	3002	rBV2	161	142	0.01%	0.001%
72	10.770	3023	3026	3029	rBV2	427	211	0.01%	0.001%
73	10.796	3030	3034	3037	rVV	340	259	0.01%	0.002%
74	10.850	3046	3051	3054	rBV2	385	350	0.02%	0.002%
75	10.918	3066	3072	3074	rBV3	645	626	0.04%	0.004%
76	11.181	3150	3154	3157	rVB3	366	246	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101222\
 Data File : VW028532.D
 Acq On : 12 Oct 2022 17:12
 Operator : SY/MD
 Sample : N5064-17ME
 Misc : 7.52g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBN6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.243	3161	3173	3200	rBV	901883	1392882	77.97%	9.799%
78	11.448	3234	3237	3238	rBV2	418	263	0.01%	0.002%
79	11.509	3254	3256	3260	rBV	243	168	0.01%	0.001%
80	11.542	3262	3266	3270	rBV2	308	302	0.02%	0.002%
81	11.615	3277	3289	3316	rBV	983821	1563818	87.54%	11.002%
82	12.008	3408	3411	3414	rBV	210	127	0.01%	0.001%
83	12.098	3435	3439	3441	rBV2	379	245	0.01%	0.002%
84	12.191	3466	3468	3477	rVB3	385	425	0.02%	0.003%
85	12.242	3477	3484	3487	rBV4	824	1011	0.06%	0.007%
86	12.352	3516	3518	3522	rBV2	280	188	0.01%	0.001%
87	12.416	3535	3538	3540	rBV	223	130	0.01%	0.001%
88	12.503	3560	3565	3566	rBV2	443	373	0.02%	0.003%
89	12.648	3606	3610	3616	rVB3	813	610	0.03%	0.004%
90	12.869	3677	3679	3682	rBV3	520	419	0.02%	0.003%
91	12.995	3715	3718	3719	rBV	241	141	0.01%	0.001%
92	13.098	3744	3750	3751	rBV	316	233	0.01%	0.002%
93	13.271	3802	3804	3806	rBV	304	150	0.01%	0.001%
94	13.361	3829	3832	3834	rBV2	229	173	0.01%	0.001%
95	13.638	3916	3918	3920	rVB	344	150	0.01%	0.001%
96	13.760	3954	3956	3959	rVB2	350	132	0.01%	0.001%
97	14.088	4056	4058	4061	rBV	461	272	0.02%	0.002%
98	14.342	4134	4137	4141	rBV3	480	401	0.02%	0.003%
99	14.943	4322	4324	4326	rBV3	617	361	0.02%	0.003%
100	15.197	4400	4403	4407	rBV4	743	737	0.04%	0.005%




Sum of corrected areas: 14214503

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101222\
Data File : VV028532.D
Acq On : 12 Oct 2022 17:12
Operator : SY/MD
Sample : N5064-17ME
Misc : 7.52g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COBN6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

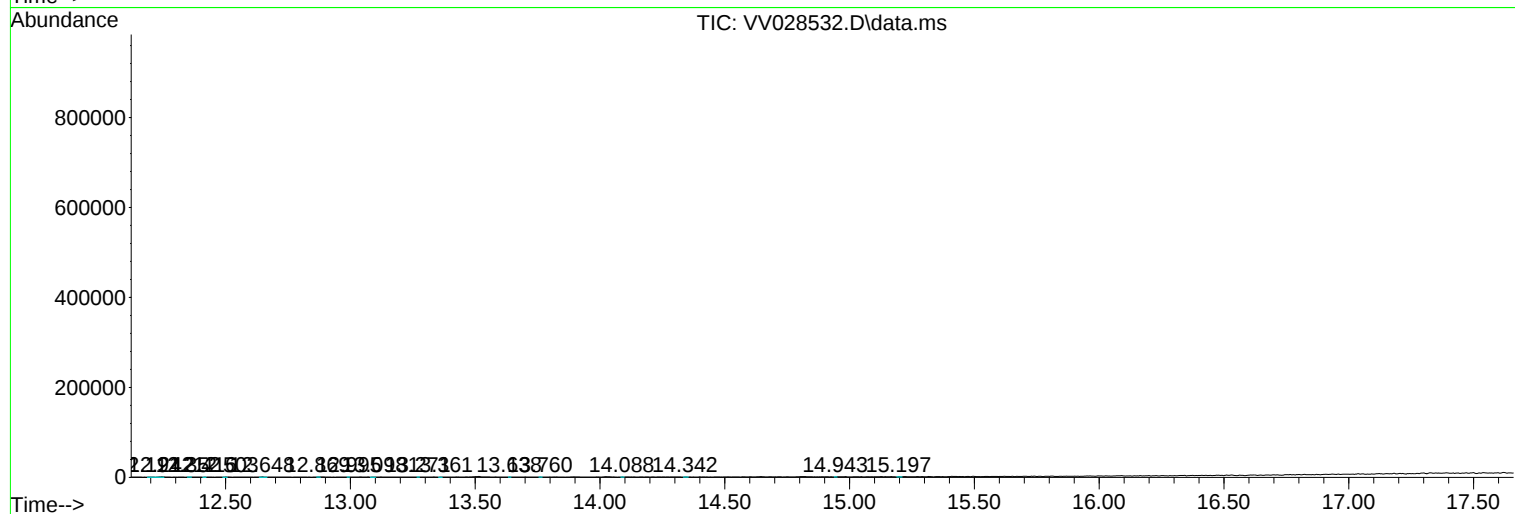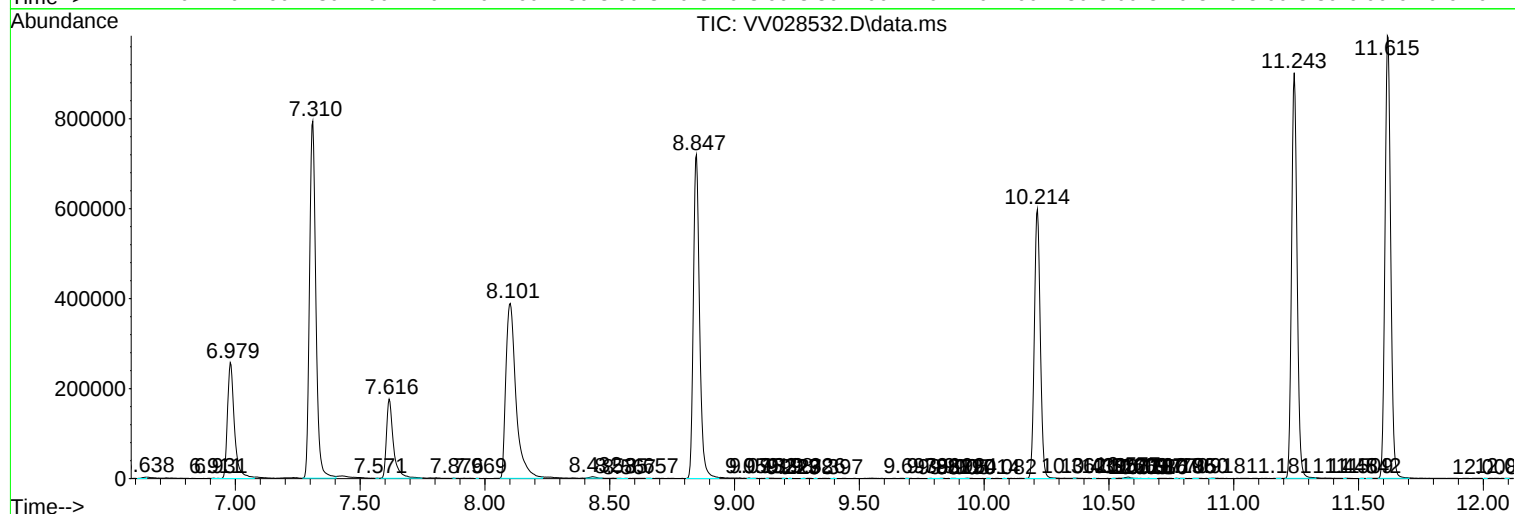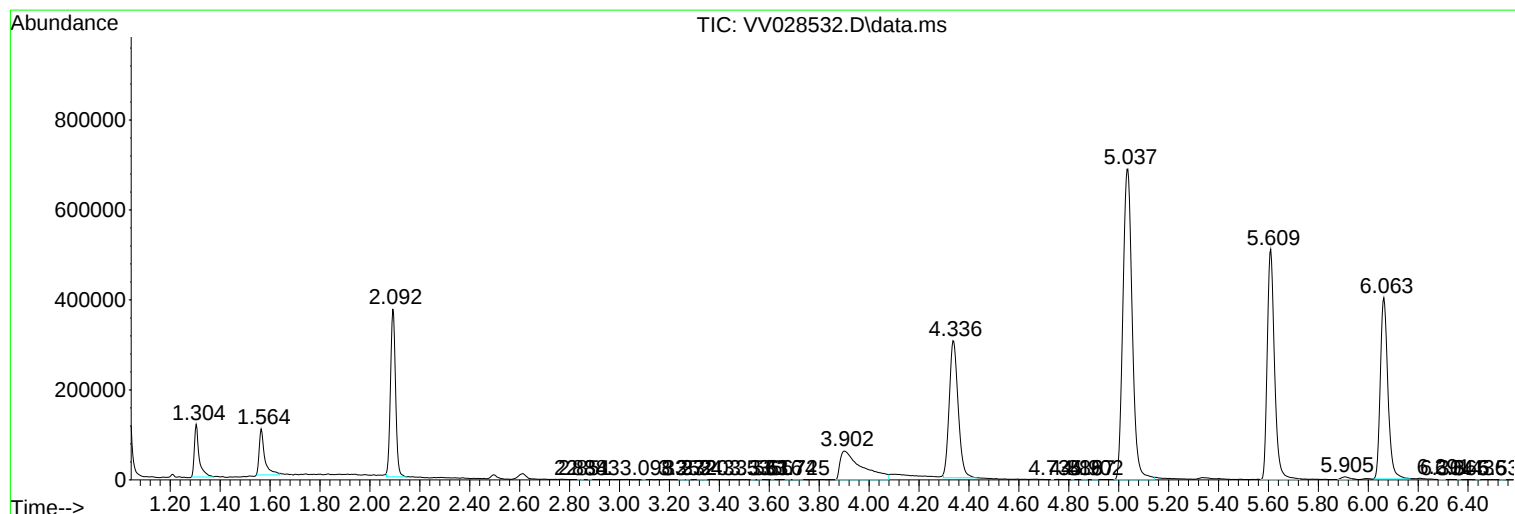

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101222\
Data File : VV028532.D
Acq On : 12 Oct 2022 17:12
Operator : SY/MD
Sample : N5064-17ME
Misc : 7.52g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BN6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101222\
Data File : VV028532.D
Acq On : 12 Oct 2022 17:12
Operator : SY/MD
Sample : N5064-17ME
Misc : 7.52g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BN6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc