
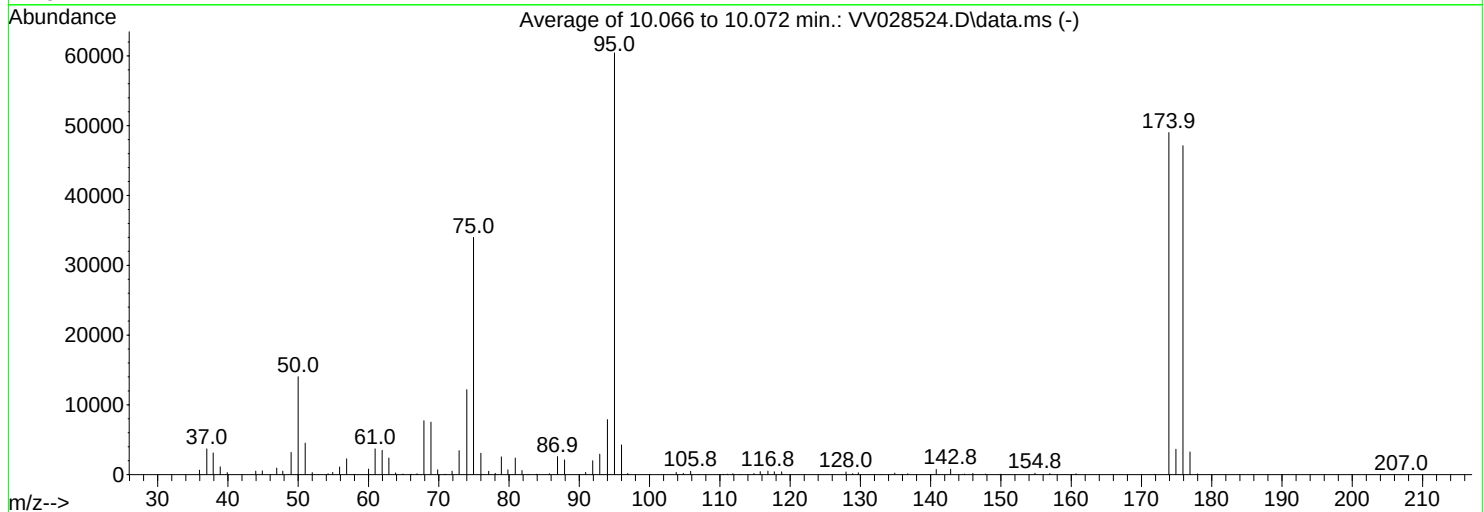


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101222\
 Data File : VV028524.D
 Acq On : 12 Oct 2022 09:01
 Operator : SY/MD
 Sample : BFB329
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB329

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis
 Last Update : Thu Oct 13 02:58:16 2022

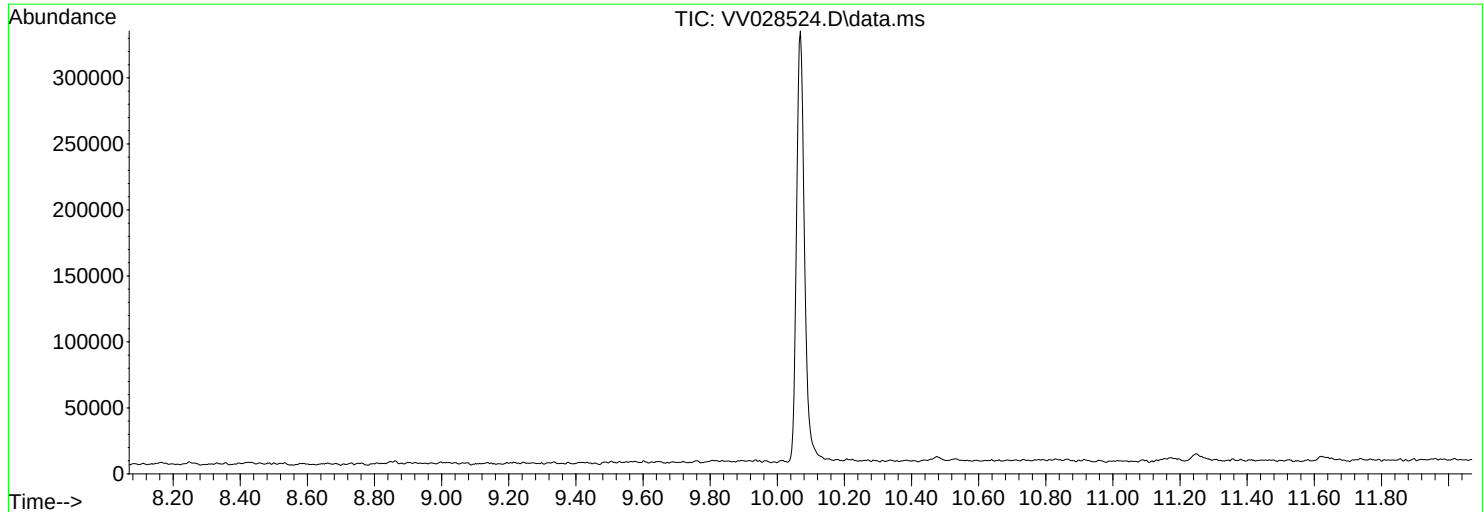

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	14042	PASS
75	95	30	80	56.2	33992	PASS
95	95	100	100	100.0	60440	PASS
96	95	5	9	7.1	4272	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.1	49027	PASS
175	174	5	9	7.5	3654	PASS
176	174	95	105	96.1	47136	PASS
177	176	5	10	6.9	3253	PASS

m/z	Abundance
37.90	108.0
38.90	301.0
39.90	2470.0
41.00	506.0
41.90	294.0
43.00	545.0
43.90	1025.0
44.90	189.0
45.90	123.0
52.80	106.0
53.90	125.0
55.00	358.0
55.90	316.0
56.90	401.0
58.00	135.0
65.70	105.0
67.00	190.0
69.00	231.0
69.80	141.0
71.00	123.0
72.90	151.0
74.90	179.0
81.10	181.0
81.90	106.0
83.90	106.0
132.70	134.0
281.00	339.0
282.10	109.0
282.90	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB329

m/z	Abundance
35.90	629.0
37.00	3630.0
38.00	3461.0
38.90	1417.0
39.90	2770.0
40.90	431.0
41.90	201.0
42.90	514.0
44.00	1533.0
44.90	744.0
46.90	1068.0
47.80	514.0
49.00	3176.0
50.00	14355.0
51.00	4450.0
52.00	282.0
53.00	134.0
54.20	138.0
54.90	681.0
55.90	1427.0
56.90	2769.0
58.00	154.0
60.00	826.0
61.00	3785.0
61.90	3595.0
62.90	2507.0
63.80	248.0
66.00	124.0
66.90	388.0
67.90	7431.0
68.90	7930.0
69.90	773.0
70.80	179.0
71.90	529.0
72.90	3761.0
74.00	12390.0
75.00	35080.0
76.00	3492.0
77.10	458.0
78.00	275.0
78.90	2764.0
79.90	642.0
80.90	2615.0
81.80	684.0
84.00	177.0
85.70	105.0
86.90	2594.0
87.90	2124.0
90.90	298.0
91.90	2126.0
92.90	3070.0
94.00	7853.0
95.00	60568.0
96.00	4209.0
96.90	244.0
103.90	307.0
104.80	197.0
105.90	483.0
107.00	104.0
111.10	100.0
111.80	105.0
112.80	102.0
114.80	191.0
115.70	456.0
116.80	556.0
117.80	434.0
118.80	393.0
127.90	387.0
128.90	136.0
129.70	312.0
133.00	105.0
134.90	211.0
136.70	145.0
140.80	702.0
142.90	771.0
144.80	145.0
146.00	193.0
147.80	146.0
154.80	208.0
156.90	159.0
160.80	116.0
173.90	48496.0
174.90	3591.0
175.90	45920.0
176.90	3322.0
177.90	107.0
281.00	283.0

Instrument :
MSVOA_V
ClientSampleId :
BFB329

m/z	Abundance
36.00	648.0
37.00	3787.0
37.90	3353.0
38.90	1446.0
39.90	2727.0
40.90	494.0
41.90	166.0
42.80	473.0
44.00	1534.0
44.90	740.0
46.90	964.0
47.80	519.0
49.00	3287.0
50.00	14591.0
51.00	4691.0
52.00	304.0
53.00	142.0
54.30	143.0
54.90	705.0
55.90	1442.0
56.90	2765.0
57.80	176.0
60.00	812.0
61.00	3826.0
62.00	3591.0
62.90	2437.0
63.90	240.0
64.90	118.0
66.10	104.0
66.80	334.0
67.90	7965.0
68.90	8017.0
69.90	863.0
70.80	199.0
71.90	514.0
73.00	3748.0
74.00	12481.0
75.00	35104.0
76.00	3134.0
77.10	497.0
78.10	294.0
78.90	2600.0
79.90	695.0
80.90	2647.0
81.90	731.0
84.00	183.0
85.80	131.0
86.90	2677.0
87.90	2170.0
90.90	340.0
91.90	2032.0
92.90	3030.0
94.00	8058.0
95.00	62296.0
96.00	4390.0
96.90	194.0
103.80	311.0
104.80	203.0
105.90	487.0
111.10	102.0
111.80	153.0
114.80	163.0
115.80	451.0
116.80	535.0
117.70	422.0
118.80	422.0
128.00	406.0
128.90	130.0
129.70	284.0
134.90	222.0
136.80	148.0
140.80	761.0
142.90	803.0
144.80	114.0
146.00	193.0
147.80	112.0
149.90	111.0
154.80	212.0
157.00	159.0
160.70	139.0
171.80	109.0
173.90	50592.0
174.90	3744.0
175.90	48720.0
176.90	3391.0
178.00	137.0
281.00	244.0

Instrument :
MSVOA_V
ClientSampleId :
BFB329

m/z	Abundance
36.00	628.0
37.00	3664.0
37.90	2846.0
38.90	1400.0
39.90	2780.0
40.90	518.0
41.90	156.0
42.80	427.0
44.00	1508.0
44.90	704.0
47.00	787.0
47.80	463.0
49.00	3080.0
50.00	13180.0
51.00	4430.0
52.00	291.0
52.90	125.0
54.30	109.0
54.90	633.0
55.90	1413.0
56.90	2461.0
57.90	200.0
60.00	774.0
60.90	3487.0
62.00	3304.0
62.90	2246.0
63.90	262.0
64.90	141.0
66.80	275.0
67.90	7756.0
68.90	7288.0
69.90	829.0
70.90	230.0
71.90	485.0
73.00	3240.0
74.00	11674.0
75.00	32328.0
76.00	2624.0
77.10	498.0
78.90	2298.0
79.80	704.0
80.90	2471.0
81.90	665.0
82.70	109.0
84.10	161.0
85.80	164.0
86.90	2518.0
87.90	2029.0
90.90	352.0
91.90	1827.0
92.90	2689.0
94.00	7787.0
95.00	58456.0
96.00	4217.0
96.90	124.0
103.70	348.0
104.80	162.0
105.80	501.0
110.50	122.0
111.90	155.0
114.90	148.0
115.80	424.0
116.90	458.0
117.70	370.0
118.80	441.0
127.90	346.0
128.90	119.0
129.70	243.0
134.90	227.0
136.80	154.0
140.80	788.0
142.80	769.0
146.00	141.0
149.90	125.0
154.90	206.0
156.90	140.0
160.60	160.0
173.90	47992.0
174.90	3628.0
175.90	46768.0
176.90	3047.0
178.00	124.0
207.00	105.0
281.00	196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB329