

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
 Data File : VV032414.D
 Acq On : 12 Oct 2023 14:10
 Operator : SY/MD
 Sample : 04851-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 12 22:38:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 12 22:36:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	108398	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	117773	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	54490	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	34931	3.962	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.200%
7) Chloroethane-d5	1.532	69	32012	4.473	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.400%
11) 1,1-Dichloroethene-d2	2.060	65	14378	3.867	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.400%
20) 2-Butanone-d5	3.806	46	77535	34.767	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	69.540%
24) Chloroform-d	4.253	84	66576	4.281	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.600%
26) 1,2-Dichloroethane-d4	4.950	65	31504	4.277	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.600%
32) Benzene-d6	4.963	84	125353	3.617	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	72.400%
36) 1,2-Dichloropropane-d6	5.992	67	40815	3.555	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	71.000%
41) Toluene-d8	7.246	98	113597	3.585	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.600%
43) trans-1,3-Dichloroprop...	7.558	79	14244	3.501	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.000%
46) 2-Hexanone-d5	8.031	63	69343	36.223	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	72.440%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	30729	3.826	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	76.600%
66) 1,2-Dichlorobenzene-d4	11.564	152	43209	4.273	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	85.400%
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	11.188	75	7062	1.218	ug/L	# 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032414.D
Acq On : 12 Oct 2023 14:10
Operator : SY/MD
Sample : 04851-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 12 22:38:20 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 12 22:36:28 2023
Response via : Initial Calibration

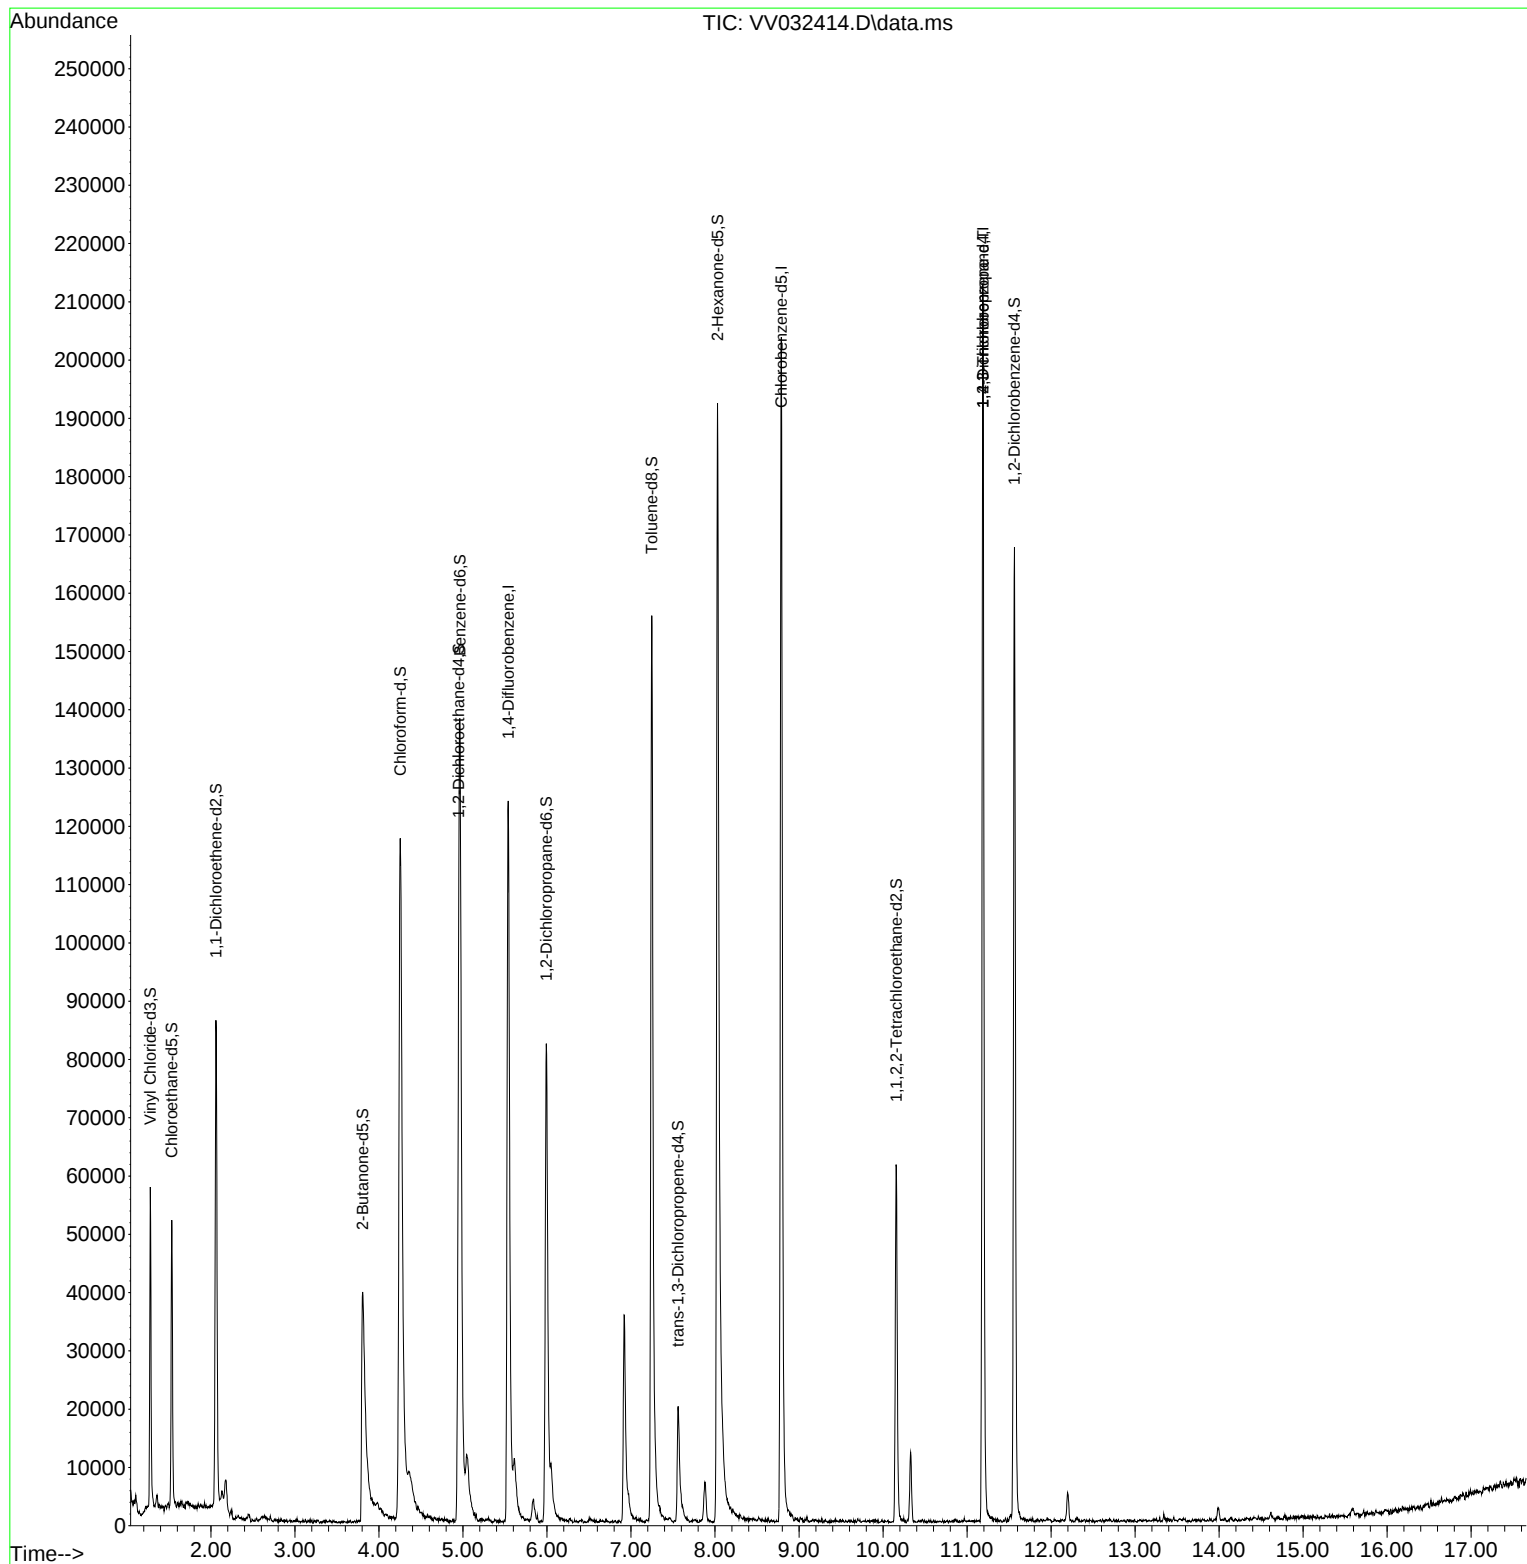

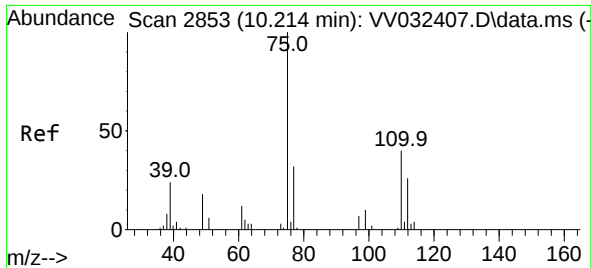

#61
 1,2,3-Trichloropropane
 Concen: 1.218 ug/L
 RT: 11.188 min Scan# 31
 Delta R.T. 0.974 min
 Lab File: VV032414.D
 Acq: 12 Oct 2023 14:10

Instrument :
 MSVOA_V
 ClientSampleId :

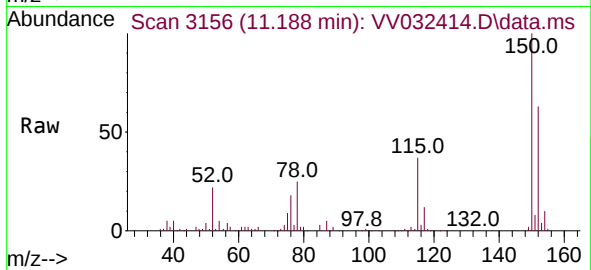

Tgt Ion: 75 Resp: 7062
 Ion Ratio Lower Upper
 75 100
 77 31.7 26.2 39.2
 110 1.6 30.6 46.0#

