

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101223\
 Data File : VW032417.D
 Acq On : 12 Oct 2023 15:23
 Operator : SY/MD
 Sample : 04326-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 12 22:39:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 12 22:36:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	101086	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	112134	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	51157	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	37611	4.575	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.400%
7) Chloroethane-d5	1.532	69	33099	4.960	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.200%
11) 1,1-Dichloroethene-d2	2.059	65	15330	4.421	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.400%
20) 2-Butanone-d5	3.805	46	93347	44.885	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.760%
24) Chloroform-d	4.256	84	69305	4.779	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
26) 1,2-Dichloroethane-d4	4.947	65	33387	4.860	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.200%
32) Benzene-d6	4.963	84	131185	3.976	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.600%
36) 1,2-Dichloropropane-d6	5.992	67	43244	3.956	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	79.200%
41) Toluene-d8	7.246	98	120686	4.000	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.000%
43) trans-1,3-Dichloroprop...	7.561	79	15488	3.998	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.000%
46) 2-Hexanone-d5	8.030	63	79717	43.737	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.480%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	35043	4.583	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.600%
66) 1,2-Dichlorobenzene-d4	11.564	152	45665	4.810	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.200%
Target Compounds						
61) 1,2,3-Trichloropropane	11.188	75	6585	1.209	ug/L	Qvalue # 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032417.D
Acq On : 12 Oct 2023 15:23
Operator : SY/MD
Sample : 04326-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 12 22:39:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 12 22:36:28 2023
Response via : Initial Calibration

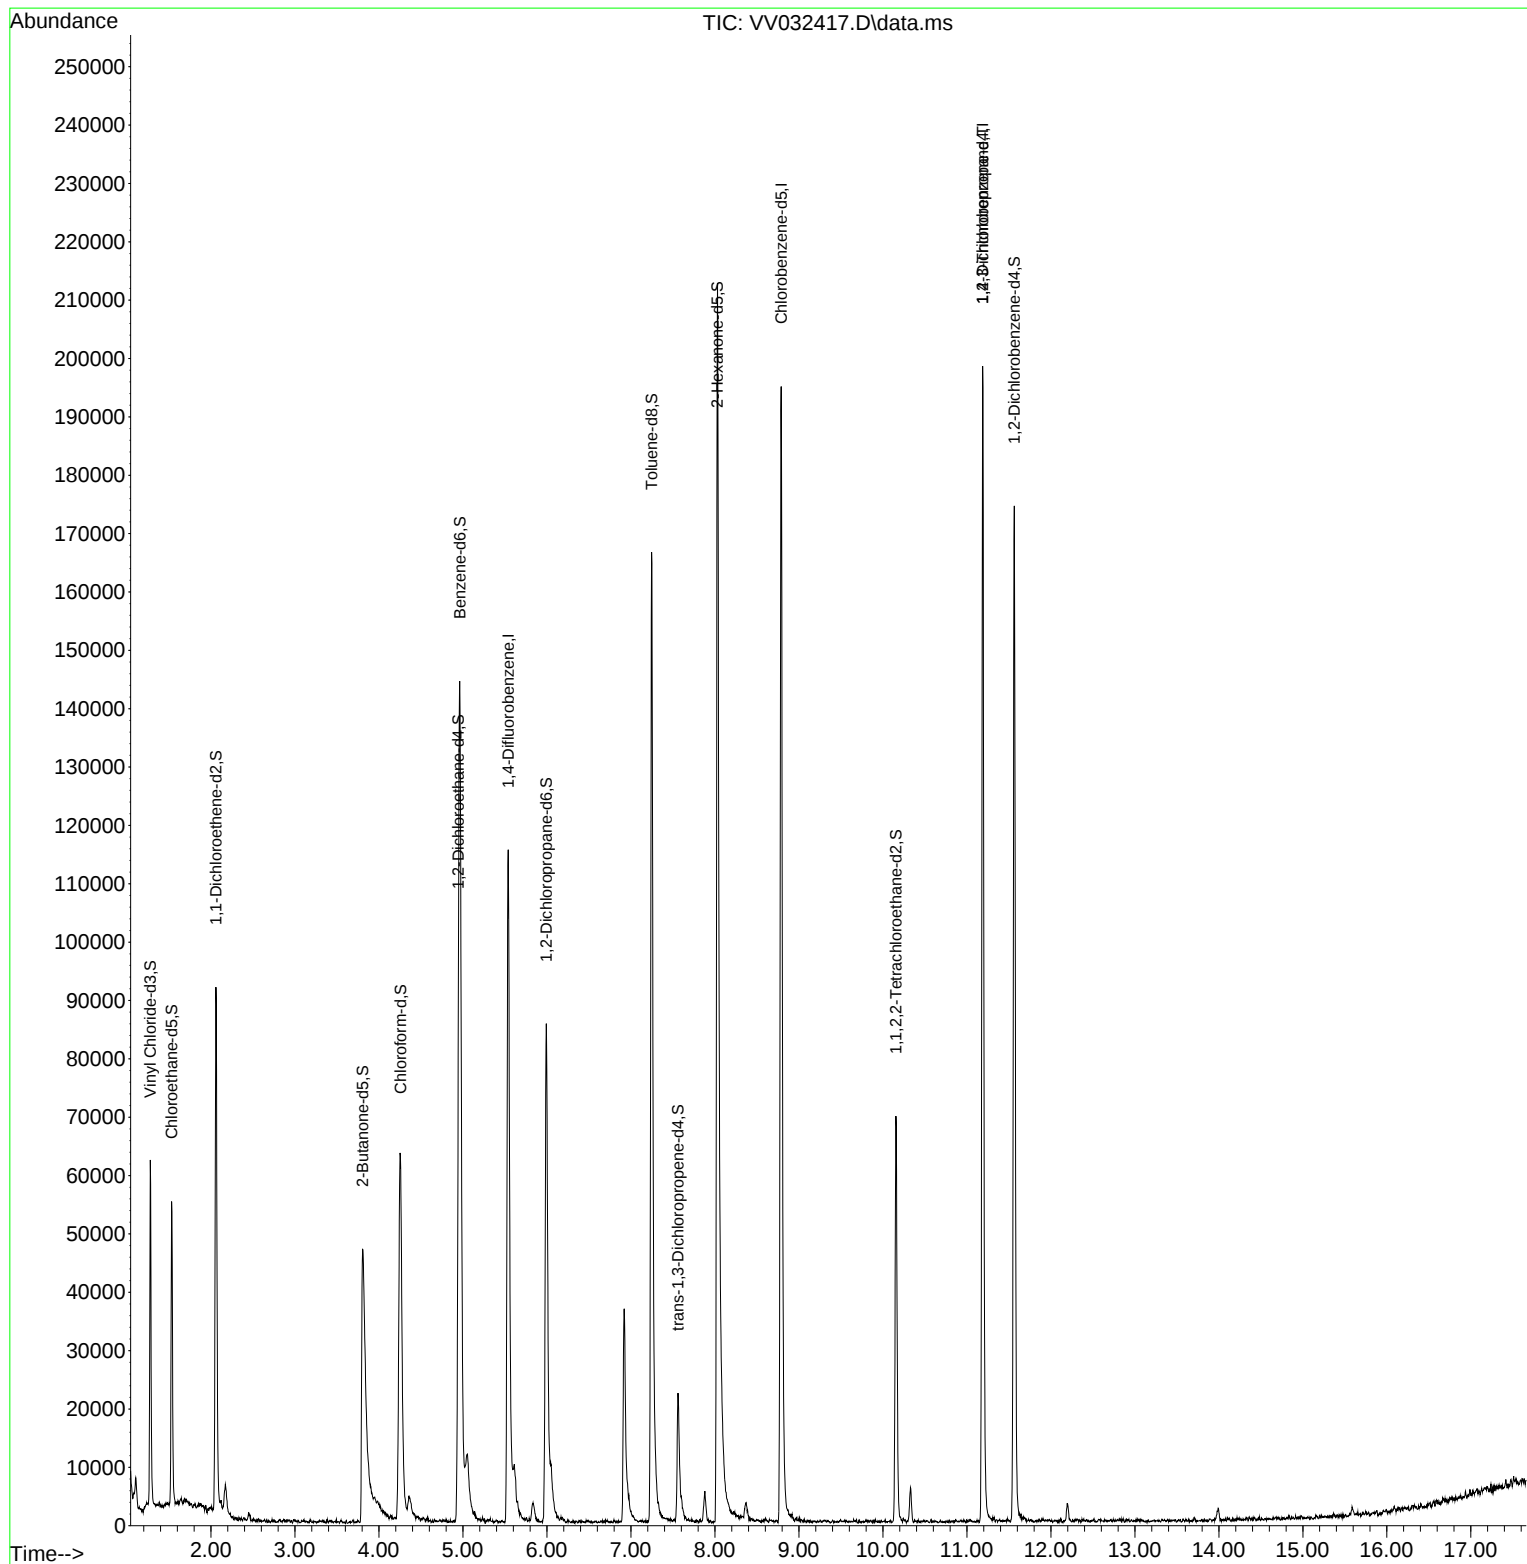

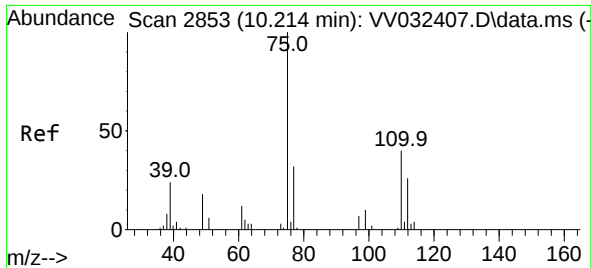

#61
 1,2,3-Trichloropropane
 Concen: 1.209 ug/L
 RT: 11.188 min Scan# 31
 Delta R.T. 0.974 min
 Lab File: VV032417.D
 Acq: 12 Oct 2023 15:23

Instrument :
 MSVOA_V
 ClientSampleId :

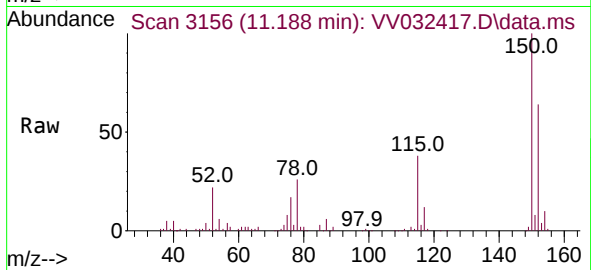

Tgt Ion: 75 Resp: 6585
 Ion Ratio Lower Upper
 75 100
 77 34.5 26.2 39.2
 110 2.8 30.6 46.0#

