

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW101223\
 Data File : VW032418.D
 Acq On : 12 Oct 2023 15:46
 Operator : SY/MD
 Sample : 04851-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 12 22:39:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 12 22:36:28 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	100643	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	111302	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	51846	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	32663	3.991	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	79.800%	
7) Chloroethane-d5	1.532	69	28620	4.308	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	86.200%	
11) 1,1-Dichloroethene-d2	2.060	65	13753	3.984	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	79.600%	
20) 2-Butanone-d5	3.809	46	91157	44.025	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	88.040%	
24) Chloroform-d	4.252	84	64152	4.443	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	88.800%	
26) 1,2-Dichloroethane-d4	4.950	65	30954	4.526	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.600%	
32) Benzene-d6	4.963	84	116697	3.563	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	71.200%	
36) 1,2-Dichloropropane-d6	5.995	67	39006	3.595	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	71.800%	
41) Toluene-d8	7.249	98	105887	3.536	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	70.800%	
43) trans-1,3-Dichloroprop...	7.561	79	13523	3.517	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	70.400%	
46) 2-Hexanone-d5	8.030	63	75869	41.937	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	83.880%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	32831	4.326	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	86.600%	
66) 1,2-Dichlorobenzene-d4	11.564	152	41710	4.335	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	86.800%	
Target Compounds						
47) Tetrachloroethene	7.911	164	5797	0.715	ug/L	97
49) Dibromochloromethane	8.182	129	3342	0.434	ug/L	90
59) Bromoform	9.673	173	916	0.243	ug/L #	93
61) 1,2,3-Trichloropropane	11.188	75	7007	1.270	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032418.D
Acq On : 12 Oct 2023 15:46
Operator : SY/MD
Sample : 04851-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 12 22:39:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 12 22:36:28 2023
Response via : Initial Calibration

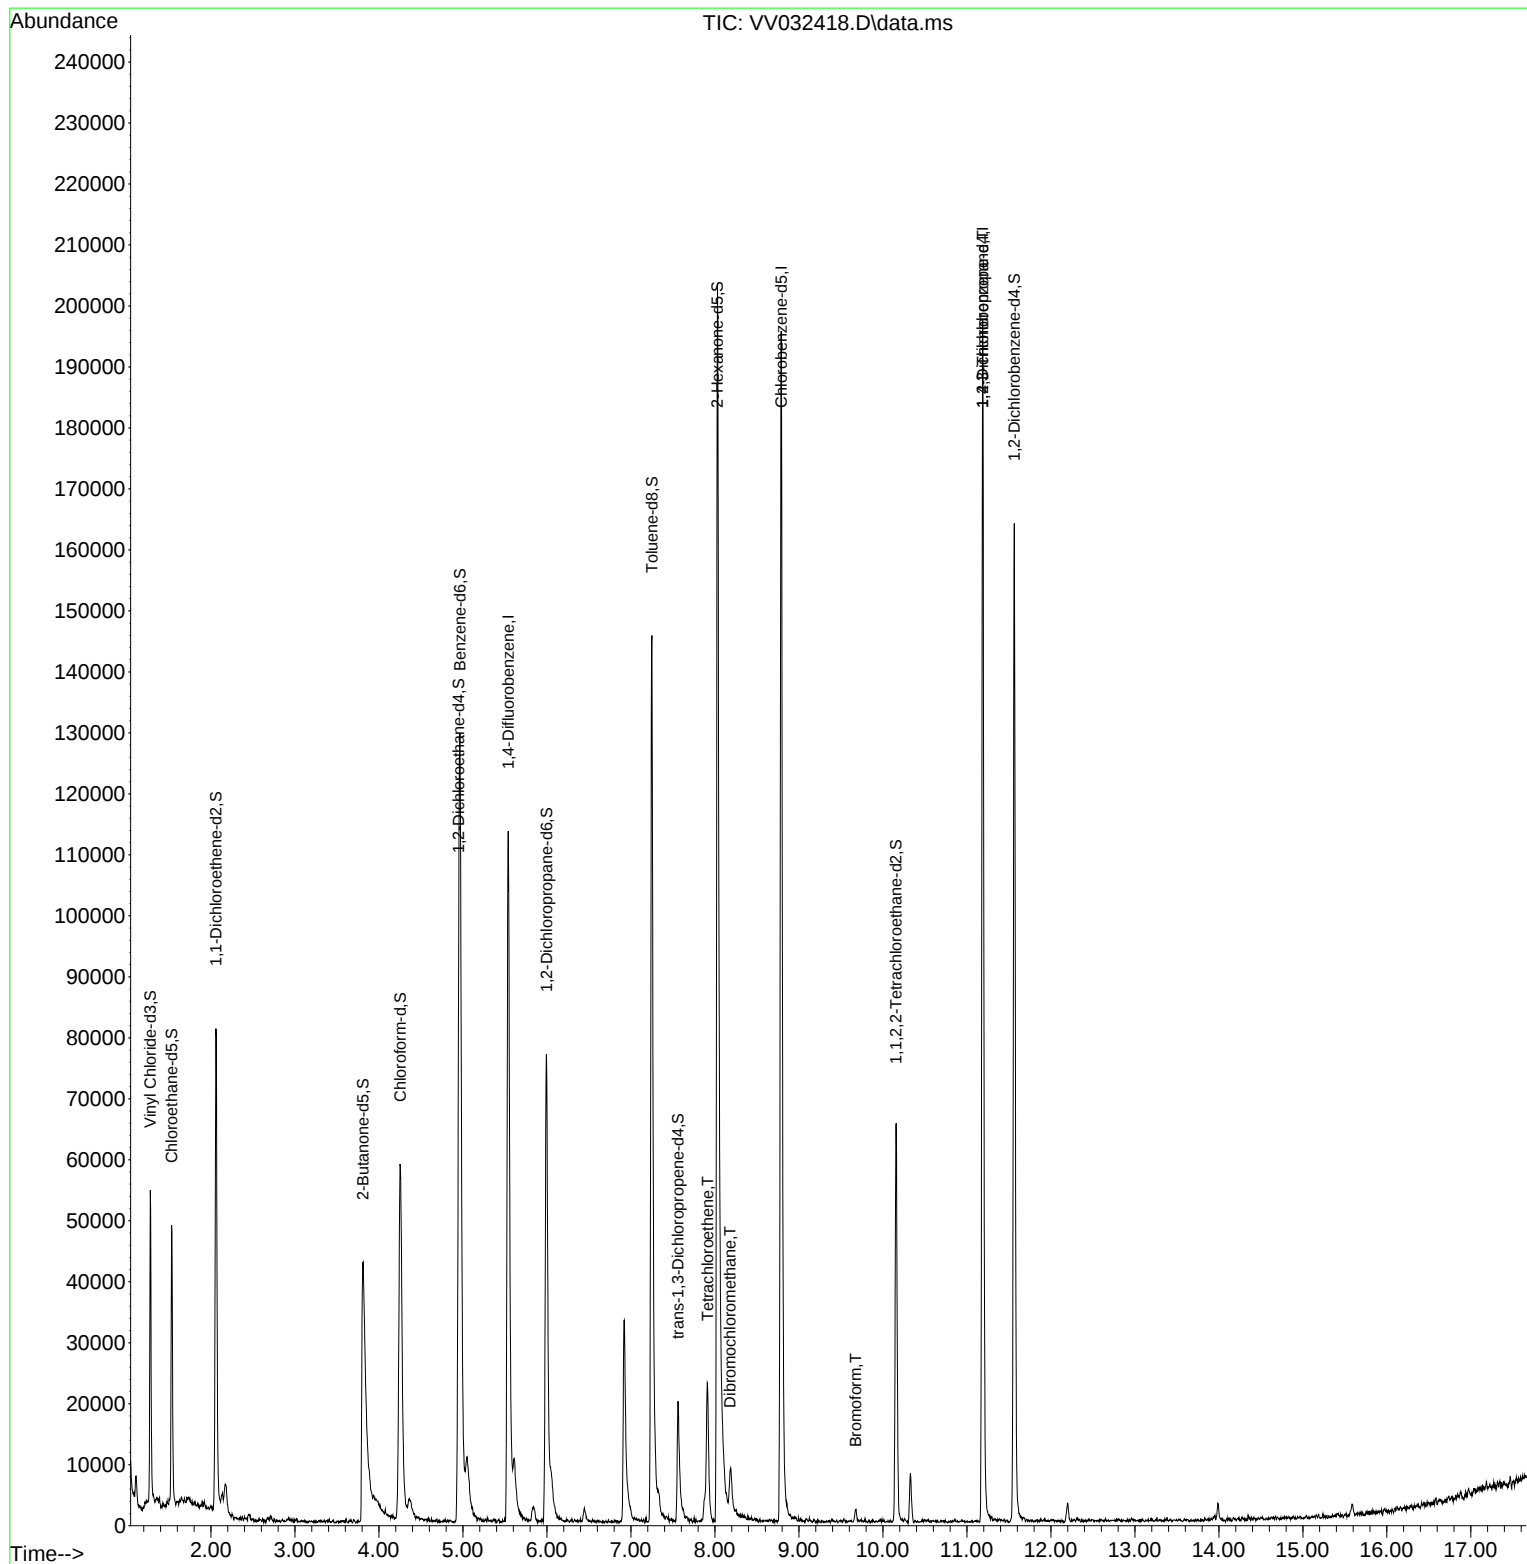



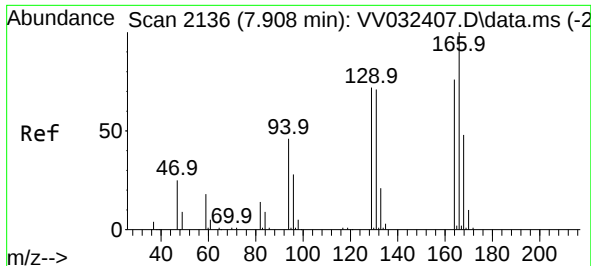


#47
Tetrachloroethene
Concen: 0.715 ug/L
RT: 7.911 min Scan# 2136
Delta R.T. 0.003 min
Lab File: VV032418.D
Acq: 12 Oct 2023 15:46

Instrument :
MSVOA_V
ClientSampleId :



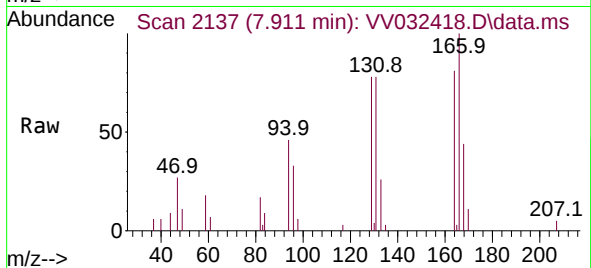



Tgt Ion:164 Resp: 5797
Ion Ratio Lower Upper
164 100
129 96.9 66.4 123.4
131 96.7 63.7 118.3
166 123.5 87.9 163.3

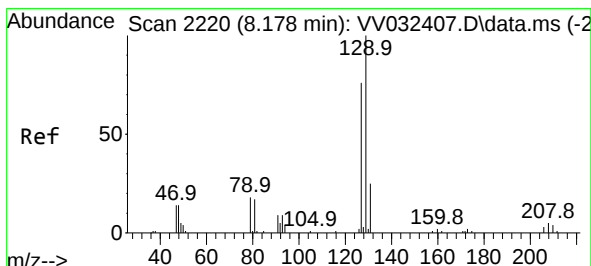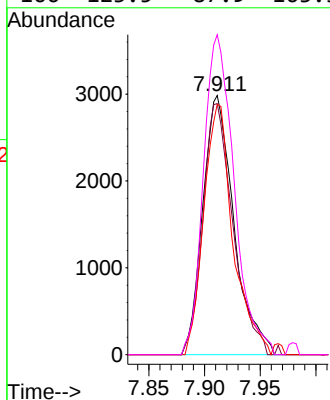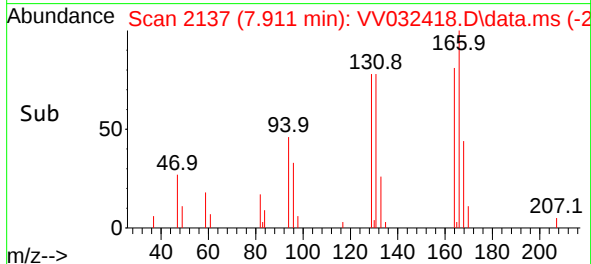

#49
Dibromochloromethane
Concen: 0.434 ug/L
RT: 8.182 min Scan# 2221
Delta R.T. 0.003 min
Lab File: VV032418.D
Acq: 12 Oct 2023 15:46

Tgt Ion:129 Resp: 3342
Ion Ratio Lower Upper
129 100
127 72.6 57.2 106.2

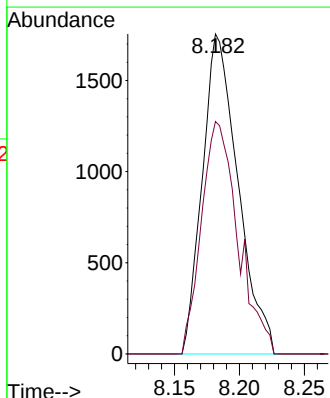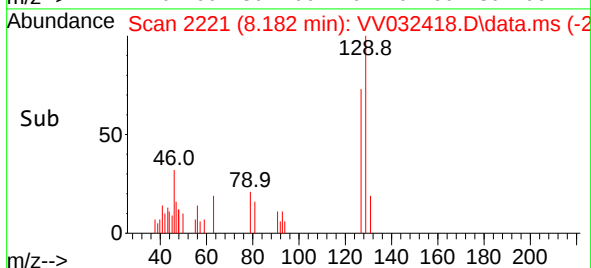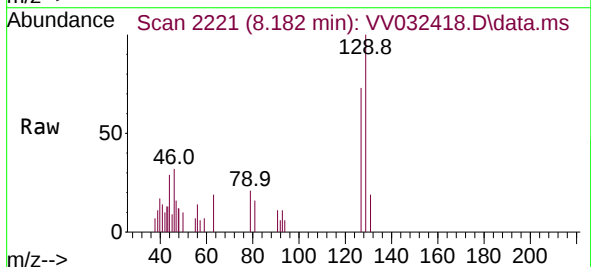

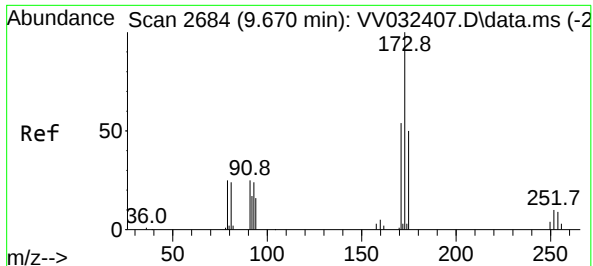

#59

Bromoform

Concen: 0.243 ug/L

RT: 9.673 min Scan# 2

Delta R.T. 0.003 min


Lab File: VV032418.D

Acq: 12 Oct 2023 15:46




Instrument :

MSVOA_V

ClientSampleId :

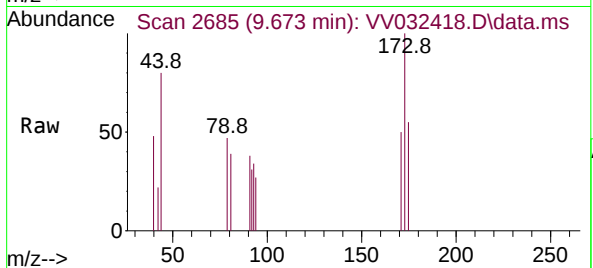

Tgt Ion:	173	Resp:	916
Ion Ratio	Lower	Upper	
173	100		
175	44.9	38.2	57.2
254	0.0	7.0	10.4

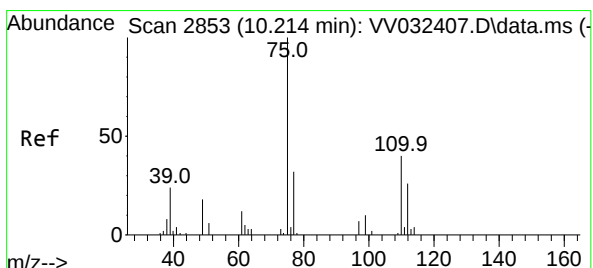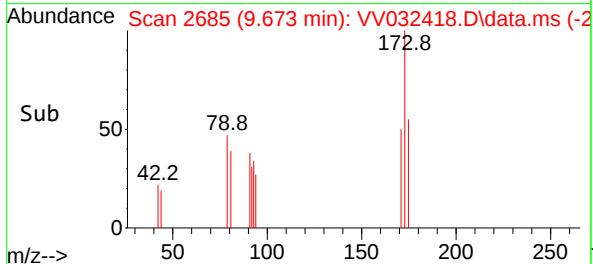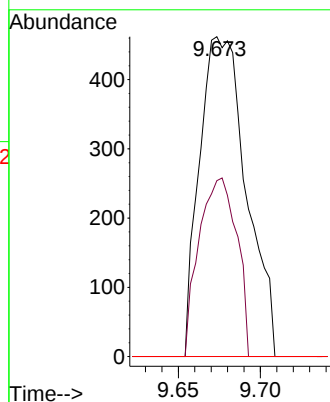

#61

1,2,3-Trichloropropane

Concen: 1.270 ug/L

RT: 11.188 min Scan# 3156

Delta R.T. 0.974 min

Lab File: VV032418.D

Acq: 12 Oct 2023 15:46

Tgt Ion:	75	Resp:	7007
Ion Ratio	Lower	Upper	
75	100		
77	34.1	26.2	39.2
110	1.3	30.6	46.0

