

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
 Data File : VV032408.D
 Acq On : 12 Oct 2023 11:00
 Operator : SY/MD
 Sample : VV1012WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK370

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032408.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	16	21	37	rVB	7131	11561	2.64%	0.339%
2	1.278	68	74	89	rVB	60351	63233	14.42%	1.853%
3	1.532	145	153	170	rVB	53472	64160	14.64%	1.880%
4	2.059	307	317	331	rBV	89180	130992	29.88%	3.839%
5	2.175	345	353	364	rVB3	6958	12819	2.92%	0.376%
6	2.449	430	438	448	rBV4	6049	9236	2.11%	0.271%
7	2.963	587	598	613	rBV6	2669	6071	1.38%	0.178%
8	3.809	852	861	896	rBV	41431	151531	34.57%	4.440%
9	4.252	984	999	1022	rBV	62731	166004	37.87%	4.864%
10	4.960	1204	1219	1238	rBV2	143371	368988	84.17%	10.813%
11	5.040	1240	1244	1266	rVB4	10940	31346	7.15%	0.919%
12	5.538	1388	1399	1415	rBV	119428	251485	57.37%	7.369%
13	5.834	1476	1491	1502	rBV9	3825	8757	2.00%	0.257%
14	5.992	1527	1540	1555	rBV	84064	181481	41.40%	5.318%
15	6.918	1816	1828	1851	rBV2	36827	80004	18.25%	2.344%
16	7.246	1917	1930	1959	rBV	168420	326260	74.43%	9.561%
17	7.561	2019	2028	2053	rBV2	22028	47583	10.85%	1.394%
18	8.030	2164	2174	2204	rBV	203445	438367	100.00%	12.846%
19	8.789	2398	2410	2431	rBV	198545	346080	78.95%	10.141%
20	10.156	2823	2835	2854	rBV	68229	110669	25.25%	3.243%
21	11.188	3146	3156	3173	rBV	202335	321963	73.45%	9.435%
22	11.564	3261	3273	3296	rBV	177623	283991	64.78%	8.322%




Sum of corrected areas: 3412581

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032408.D
Acq On : 12 Oct 2023 11:00
Operator : SY/MD
Sample : VV1012WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK370

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

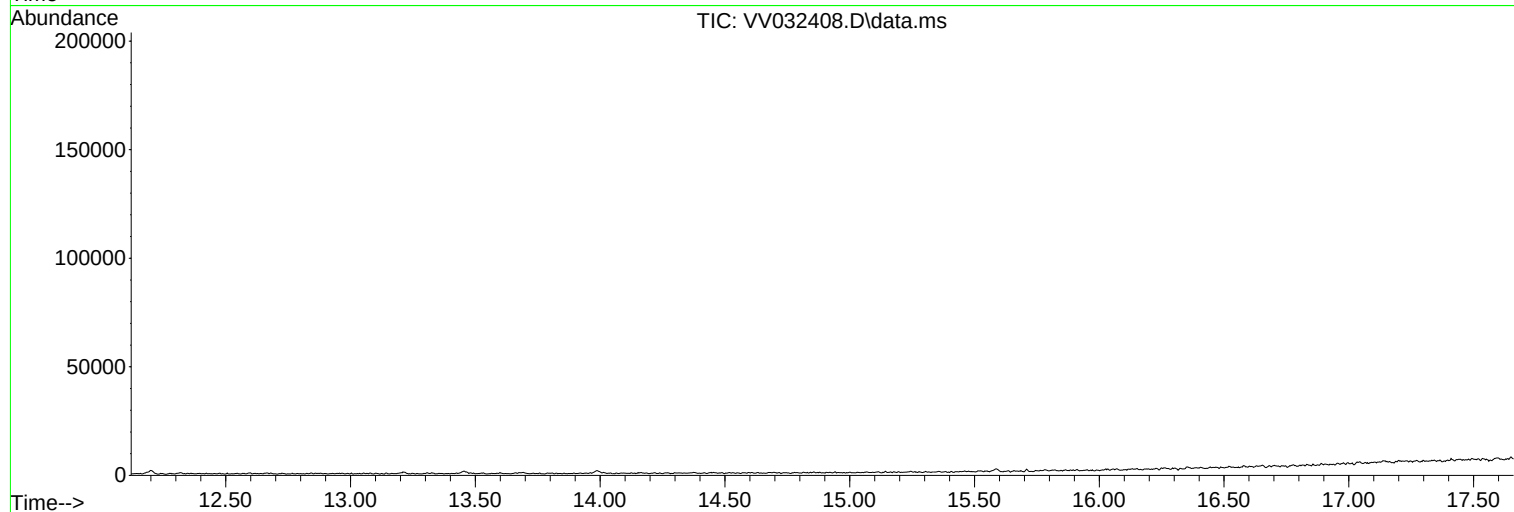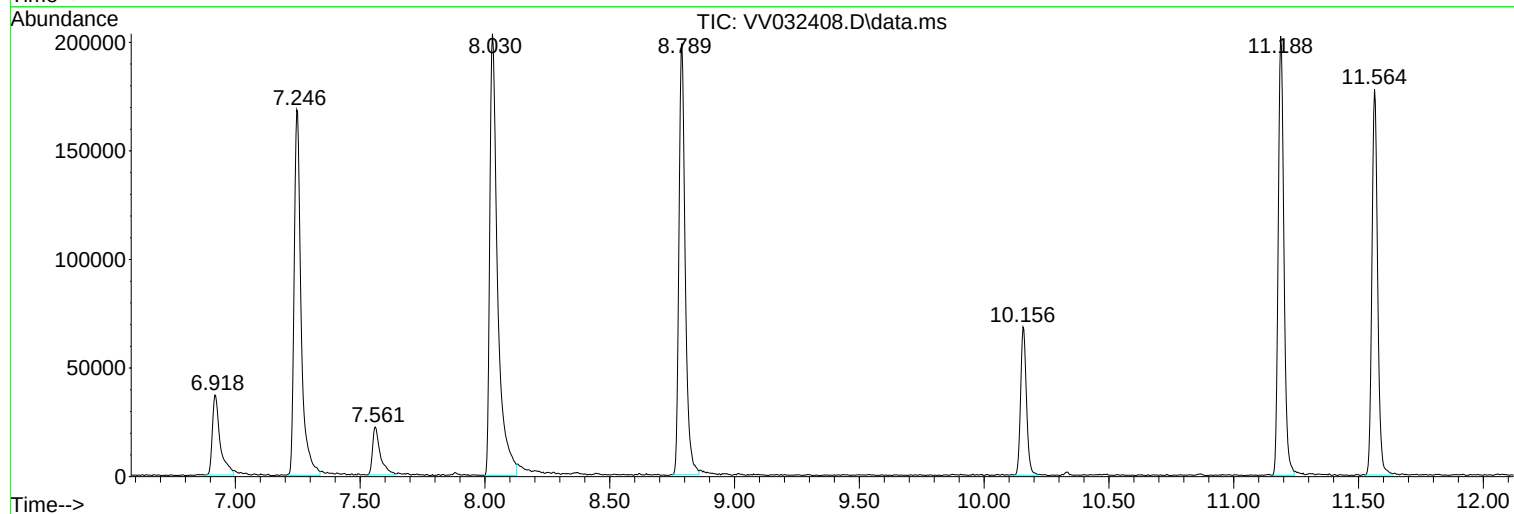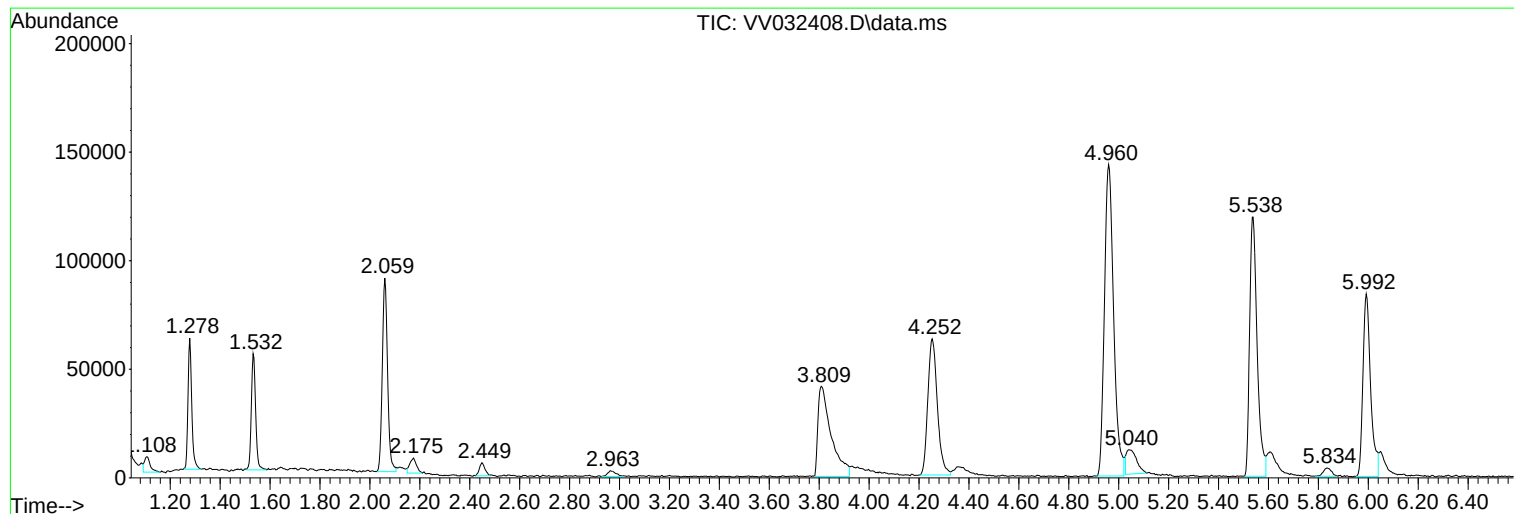

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032408.D
Acq On : 12 Oct 2023 11:00
Operator : SY/MD
Sample : VV1012WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK370

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032408.D
Acq On : 12 Oct 2023 11:00
Operator : SY/MD
Sample : VV1012WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK370

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------