

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
 Data File : VV032409.D
 Acq On : 12 Oct 2023 11:29
 Operator : SY/MD
 Sample : 04826-03DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCJV0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032409.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	18	21	35	rVB	6546	8601	1.52%	0.227%
2	1.278	67	74	90	rVB	60600	64820	11.46%	1.713%
3	1.532	146	153	167	rVB	51026	59447	10.51%	1.571%
4	2.060	307	317	331	rBV	84083	125008	22.10%	3.303%
5	2.172	346	352	365	rVB3	6901	12615	2.23%	0.333%
6	2.449	428	438	449	rBV	11671	19641	3.47%	0.519%
7	2.976	588	602	615	rBV6	2272	5720	1.01%	0.151%
8	3.805	850	860	885	rBV3	48378	155282	27.45%	4.103%
9	4.252	982	999	1023	rBV	61093	167110	29.54%	4.416%
10	4.960	1200	1219	1238	rBV3	132932	345842	61.14%	9.139%
11	5.538	1388	1399	1416	rBV	113802	242139	42.81%	6.399%
12	5.834	1478	1491	1504	rBV	280636	565621	100.00%	14.947%
13	5.992	1529	1540	1553	rBV	75288	156201	27.62%	4.128%
14	6.918	1816	1828	1856	rBV2	34025	78356	13.85%	2.071%
15	7.246	1919	1930	1967	rBV	154839	307037	54.28%	8.113%
16	7.561	2019	2028	2043	rBV3	19993	41391	7.32%	1.094%
17	8.030	2164	2174	2204	rBV	190068	406725	71.91%	10.748%
18	8.789	2393	2410	2434	rBV	196127	339486	60.02%	8.971%
19	10.156	2824	2835	2854	rBV	65037	103665	18.33%	2.739%
20	11.191	3145	3157	3175	rBV	197357	314000	55.51%	8.297%
21	11.564	3262	3273	3295	rBV	163720	265569	46.95%	7.018%




Sum of corrected areas: 3784276

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032409.D
Acq On : 12 Oct 2023 11:29
Operator : SY/MD
Sample : 04826-03DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJV0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

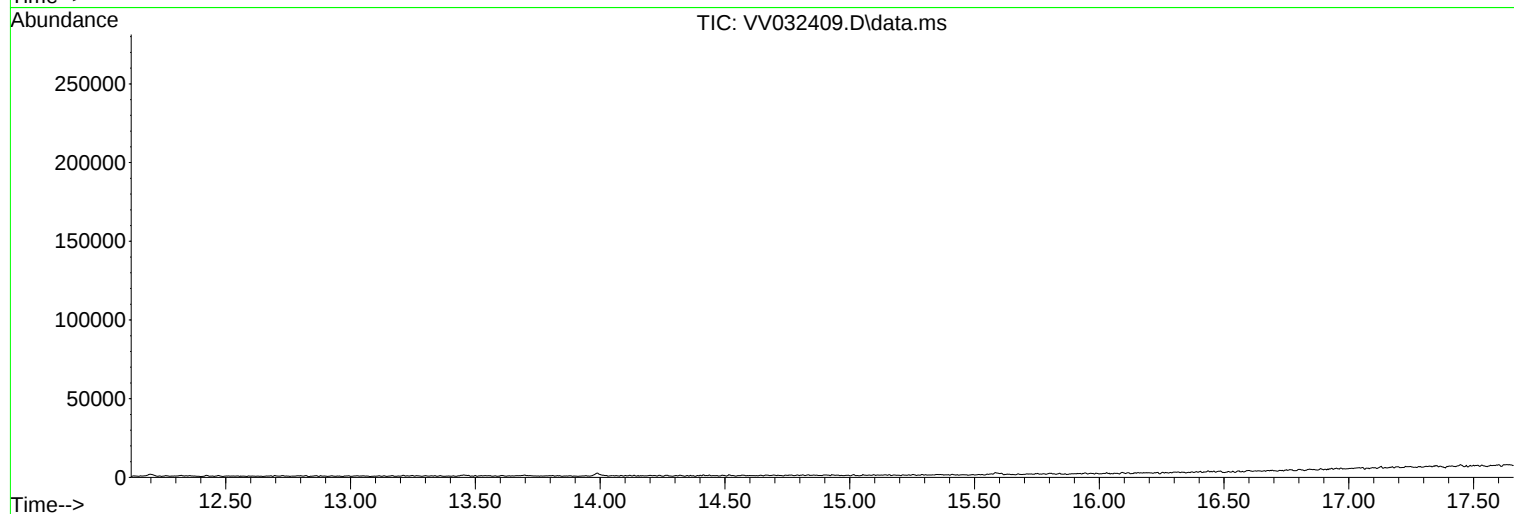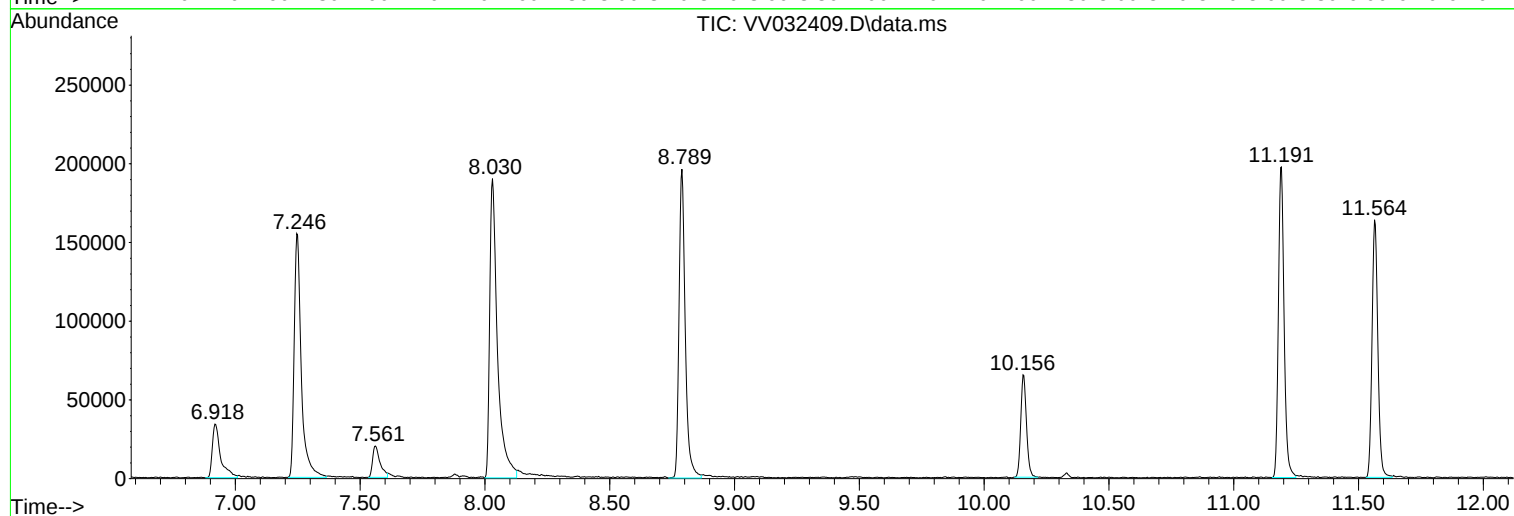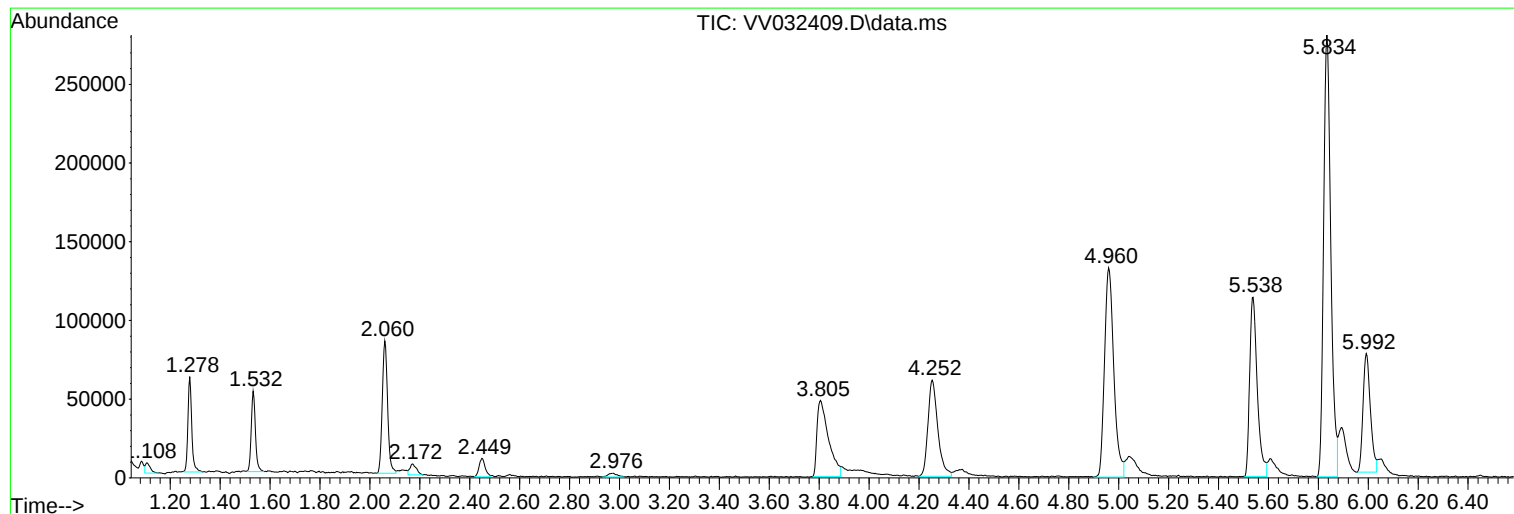

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032409.D
Acq On : 12 Oct 2023 11:29
Operator : SY/MD
Sample : 04826-03DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJV0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032409.D
Acq On : 12 Oct 2023 11:29
Operator : SY/MD
Sample : 04826-03DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCJV0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------