

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
 Data File : VV032411.D
 Acq On : 12 Oct 2023 12:59
 Operator : SY/MD
 Sample : 04851-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B07

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032411.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	17	23	33	rVB	4923	7163	1.56%	0.206%
2	1.278	67	74	90	rVB	57100	62226	13.56%	1.789%
3	1.532	146	153	166	rVB	49806	58514	12.75%	1.682%
4	2.060	307	317	332	rBV	84216	124834	27.20%	3.589%
5	2.182	347	355	367	rVB2	7510	14137	3.08%	0.406%
6	3.806	851	860	889	rBV	46277	153179	33.37%	4.403%
7	4.253	984	999	1024	rBV2	60872	167660	36.53%	4.820%
8	4.372	1028	1036	1058	rVB6	5136	13678	2.98%	0.393%
9	4.960	1202	1219	1238	rBV2	142342	364721	79.47%	10.485%
10	5.053	1242	1248	1264	rVB2	10810	25174	5.48%	0.724%
11	5.539	1387	1399	1417	rBV	115950	246188	53.64%	7.077%
12	5.838	1478	1492	1498	rBV8	2804	5820	1.27%	0.167%
13	5.992	1525	1540	1555	rBV	82196	177454	38.66%	5.101%
14	6.439	1670	1679	1689	rBV3	7949	15410	3.36%	0.443%
15	6.921	1817	1829	1858	rBV	35209	82143	17.90%	2.361%
16	7.246	1919	1930	1961	rBV	163310	323510	70.49%	9.300%
17	7.561	2019	2028	2039	rBV2	21125	39505	8.61%	1.136%
18	7.912	2129	2137	2150	rVB3	20277	37137	8.09%	1.068%
19	8.031	2162	2174	2204	rBV	217914	458964	100.00%	13.194%
20	8.182	2212	2221	2236	rVB3	13811	29027	6.32%	0.834%
21	8.789	2398	2410	2429	rBV	192353	338079	73.66%	9.719%
22	9.670	2676	2684	2695	rBV6	4226	7152	1.56%	0.206%
23	10.159	2825	2836	2853	rBV	70115	114265	24.90%	3.285%
24	10.330	2879	2889	2899	rBV2	9349	14427	3.14%	0.415%
25	11.188	3144	3156	3175	rBV	198753	314966	68.63%	9.054%
26	11.564	3261	3273	3289	rBV	173133	278450	60.67%	8.005%
27	12.194	3464	3469	3480	rVB	3170	4840	1.05%	0.139%




Sum of corrected areas: 3478623

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032411.D
Acq On : 12 Oct 2023 12:59
Operator : SY/MD
Sample : 04851-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

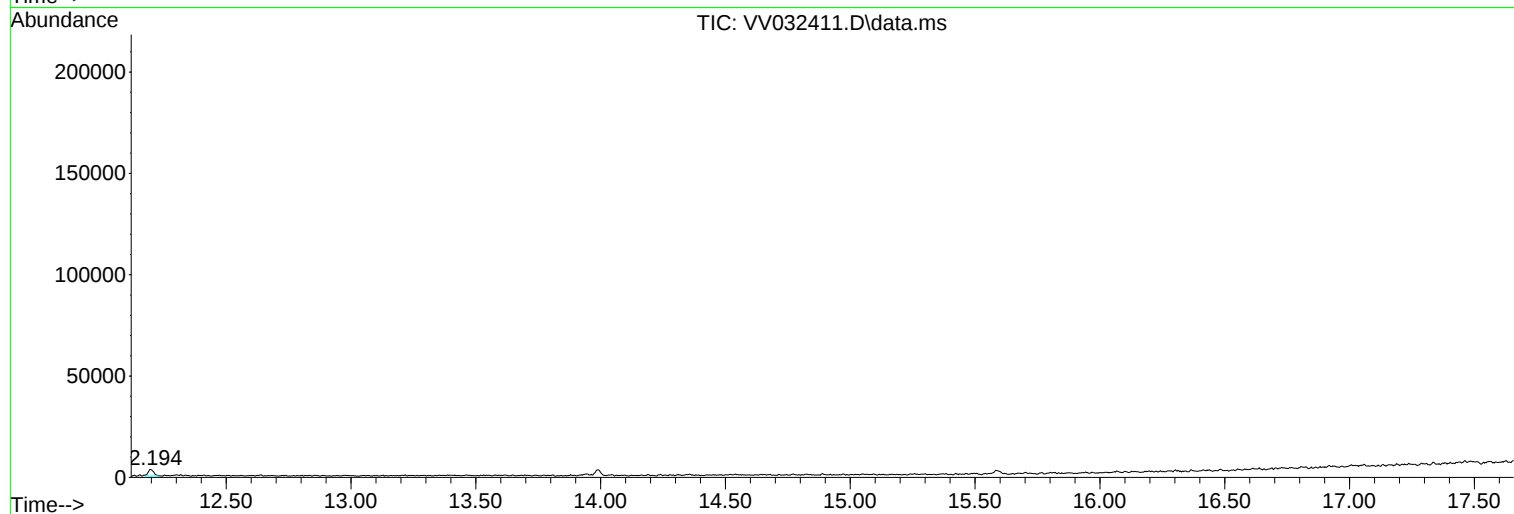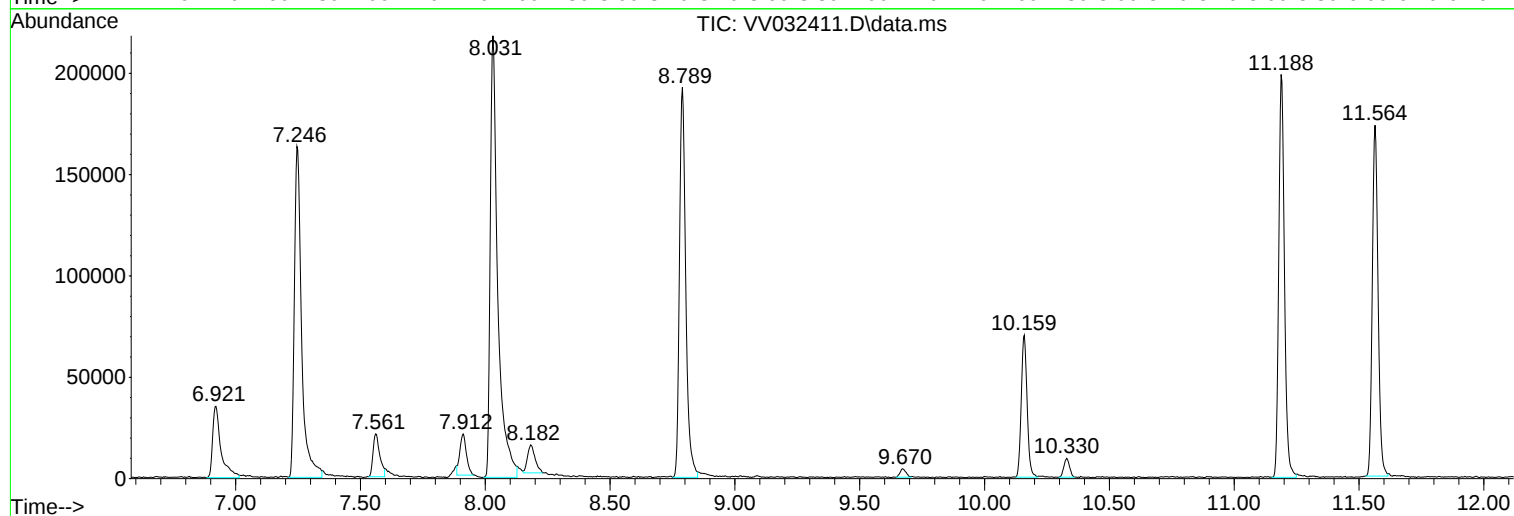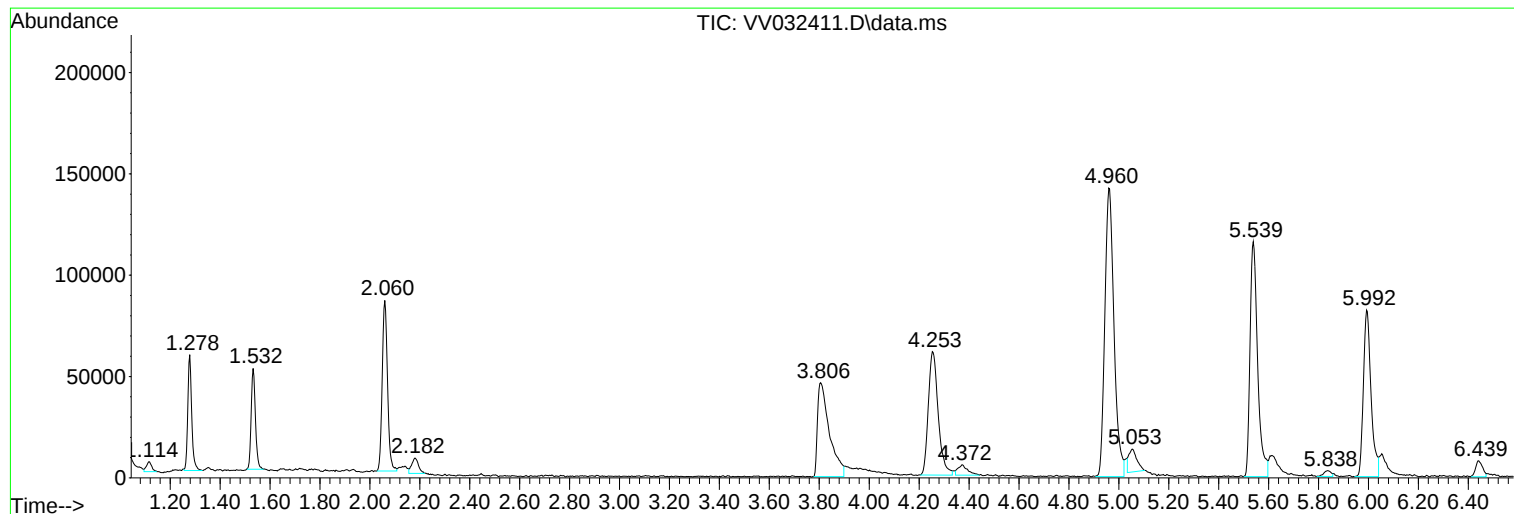

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032411.D
Acq On : 12 Oct 2023 12:59
Operator : SY/MD
Sample : 04851-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032411.D
Acq On : 12 Oct 2023 12:59
Operator : SY/MD
Sample : 04851-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------