

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
 Data File : VV032414.D
 Acq On : 12 Oct 2023 14:10
 Operator : SY/MD
 Sample : 04851-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032414.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	87	rBV	54816	57443	13.18%	1.658%
2	1.532	146	153	164	rBV	48944	57499	13.19%	1.659%
3	2.060	308	317	330	rBV	82903	120336	27.61%	3.473%
4	2.175	346	353	368	rVB3	6102	13072	3.00%	0.377%
5	3.806	851	860	893	rBV2	39332	130388	29.92%	3.763%
6	4.253	982	999	1026	rBV4	116806	336580	77.23%	9.713%
7	4.960	1201	1219	1239	rBV2	137956	358252	82.20%	10.338%
8	5.539	1387	1399	1416	rBV	123616	262213	60.17%	7.567%
9	5.838	1482	1492	1504	rBV7	3561	7435	1.71%	0.215%
10	5.992	1526	1540	1554	rBV	82043	172141	39.50%	4.967%
11	6.918	1818	1828	1844	rBV2	35319	70704	16.22%	2.040%
12	7.246	1919	1930	1957	rBV	155258	301521	69.18%	8.701%
13	7.561	2018	2028	2043	rBV	19749	41139	9.44%	1.187%
14	7.879	2117	2127	2138	rVB3	6654	12250	2.81%	0.353%
15	8.031	2161	2174	2219	rBV2	192001	435820	100.00%	12.576%
16	8.789	2399	2410	2434	rBV	203216	358583	82.28%	10.348%
17	10.156	2824	2835	2854	rBV2	61312	100988	23.17%	2.914%
18	10.329	2879	2889	2899	rVB	11928	18291	4.20%	0.528%
19	11.188	3146	3156	3173	rBV	212557	333257	76.47%	9.617%
20	11.564	3262	3273	3297	rVB2	166789	269299	61.79%	7.771%
21	12.198	3459	3470	3479	rBV2	4874	8186	1.88%	0.236%




Sum of corrected areas: 3465397

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032414.D
Acq On : 12 Oct 2023 14:10
Operator : SY/MD
Sample : 04851-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

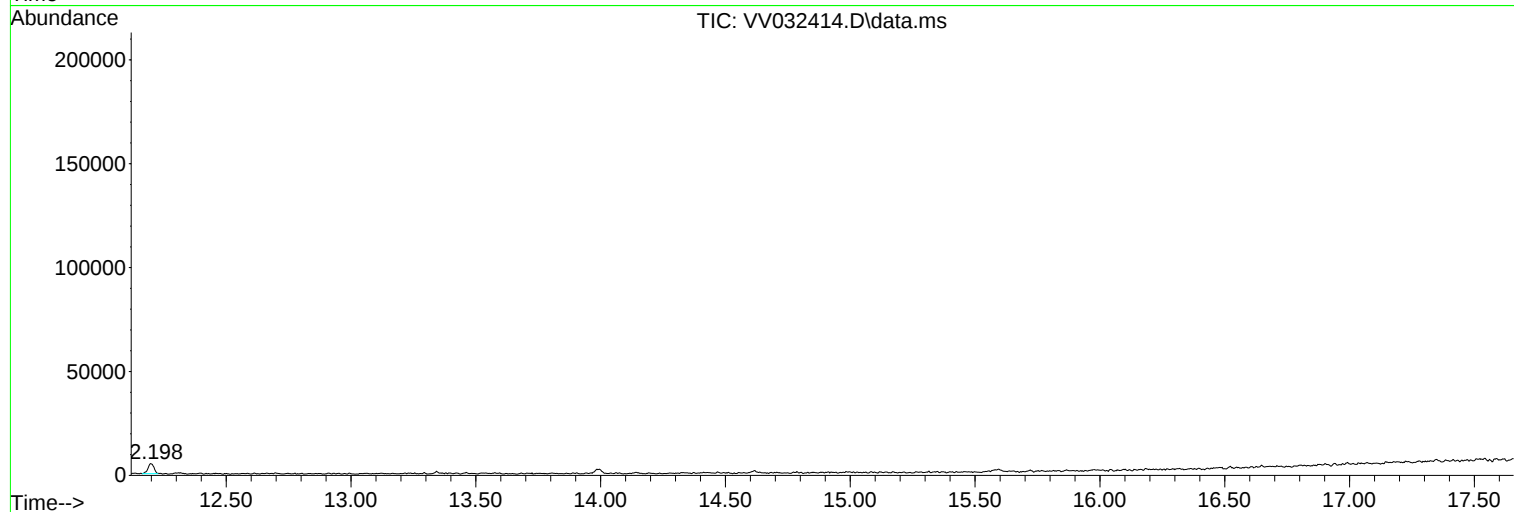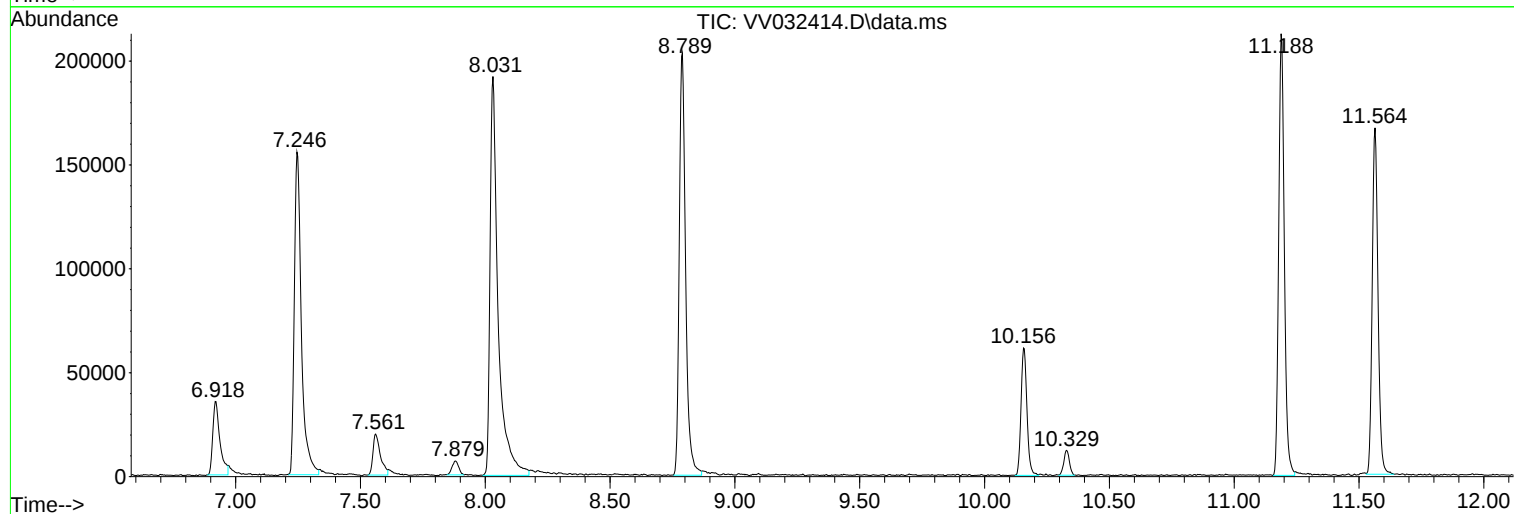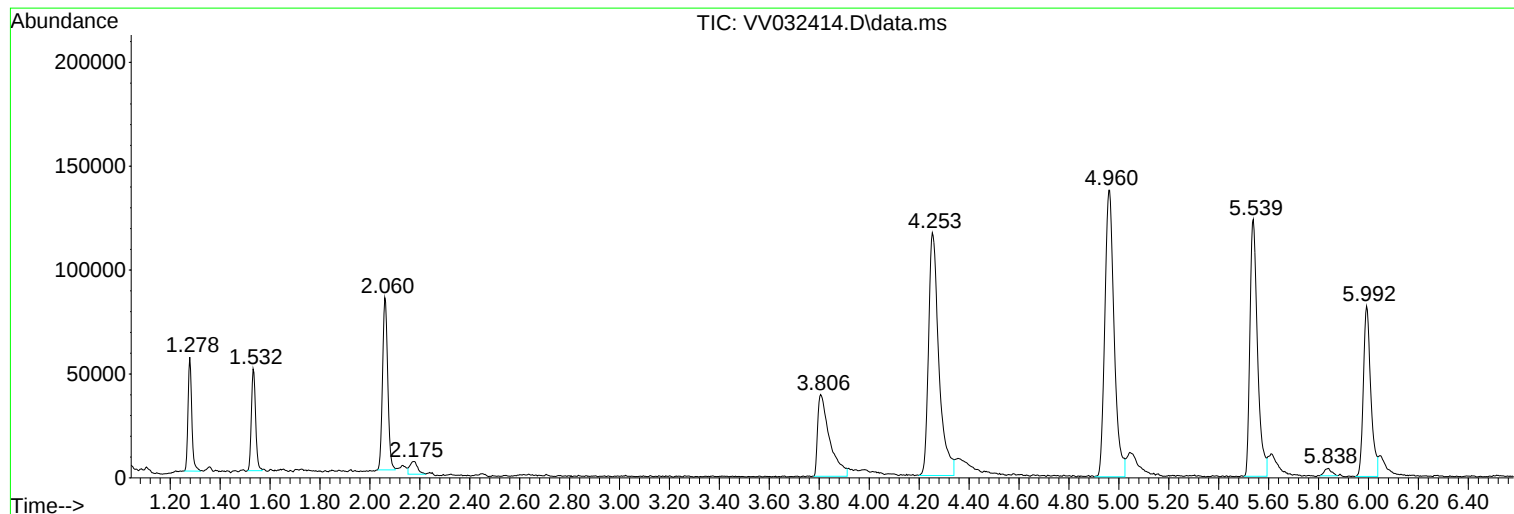

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032414.D
Acq On : 12 Oct 2023 14:10
Operator : SY/MD
Sample : 04851-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032414.D
Acq On : 12 Oct 2023 14:10
Operator : SY/MD
Sample : 04851-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------