

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
 Data File : VV032415.D
 Acq On : 12 Oct 2023 14:34
 Operator : SY/MD
 Sample : 04851-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B11

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032415.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rBV	55847	59523	13.06%	1.729%
2	1.532	146	153	163	rBV	48670	56516	12.40%	1.642%
3	2.060	306	317	329	rBV	85486	125669	27.57%	3.651%
4	2.172	344	352	364	rVB3	5050	10387	2.28%	0.302%
5	2.449	430	438	448	rBV3	5571	8829	1.94%	0.257%
6	2.516	448	459	470	rVB	11367	19893	4.36%	0.578%
7	3.805	851	860	895	rBV2	45679	157045	34.45%	4.563%
8	4.256	983	1000	1025	rBV2	65859	199390	43.74%	5.793%
9	4.960	1203	1219	1238	rBV2	141116	362414	79.51%	10.530%
10	5.539	1385	1399	1416	rBV	124290	261948	57.47%	7.611%
11	5.834	1480	1491	1502	rBV9	3882	8802	1.93%	0.256%
12	5.992	1528	1540	1558	rBV2	83714	183124	40.18%	5.321%
13	6.918	1819	1828	1856	rBV2	35863	78025	17.12%	2.267%
14	7.246	1919	1930	1955	rBV	159409	307659	67.50%	8.939%
15	7.561	2019	2028	2049	rBV	22309	46153	10.13%	1.341%
16	7.882	2116	2128	2136	rBV2	3958	7564	1.66%	0.220%
17	8.030	2164	2174	2212	rBV	209641	455803	100.00%	13.243%
18	8.789	2398	2410	2436	rBV	203713	361717	79.36%	10.510%
19	10.159	2825	2836	2852	rBV	67123	108840	23.88%	3.162%
20	10.326	2876	2888	2900	rBV3	5904	9983	2.19%	0.290%
21	11.188	3142	3156	3176	rBV	209216	334458	73.38%	9.718%
22	11.564	3262	3273	3291	rVB2	172179	278011	60.99%	8.078%




Sum of corrected areas: 3441753

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032415.D
Acq On : 12 Oct 2023 14:34
Operator : SY/MD
Sample : 04851-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

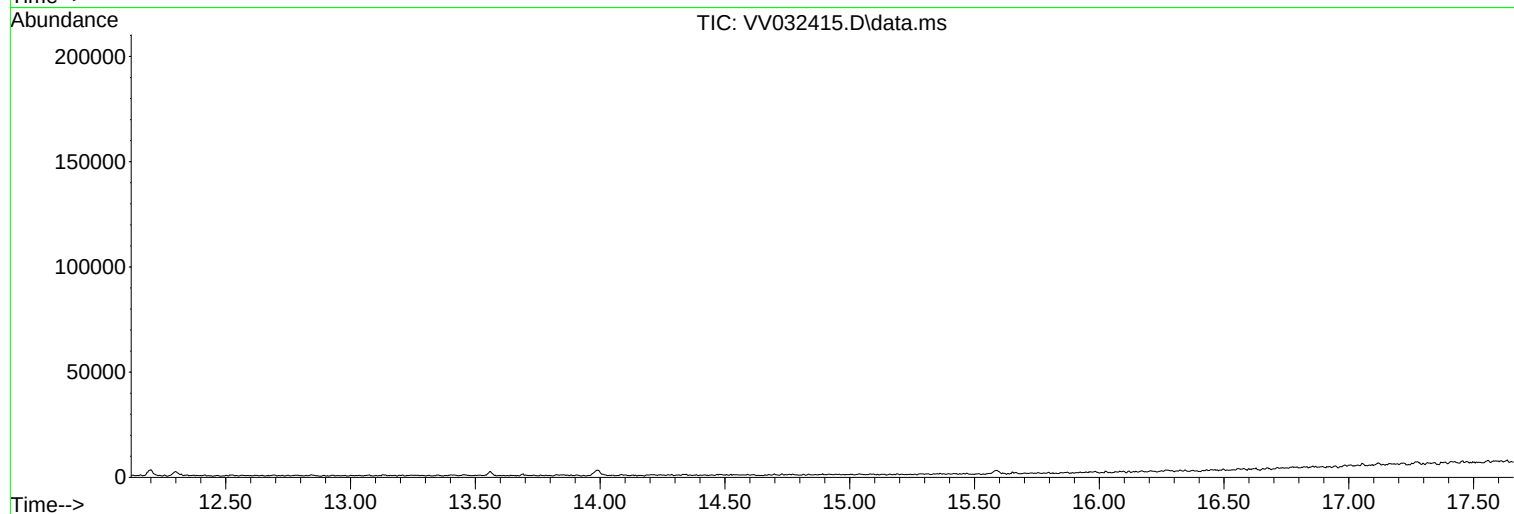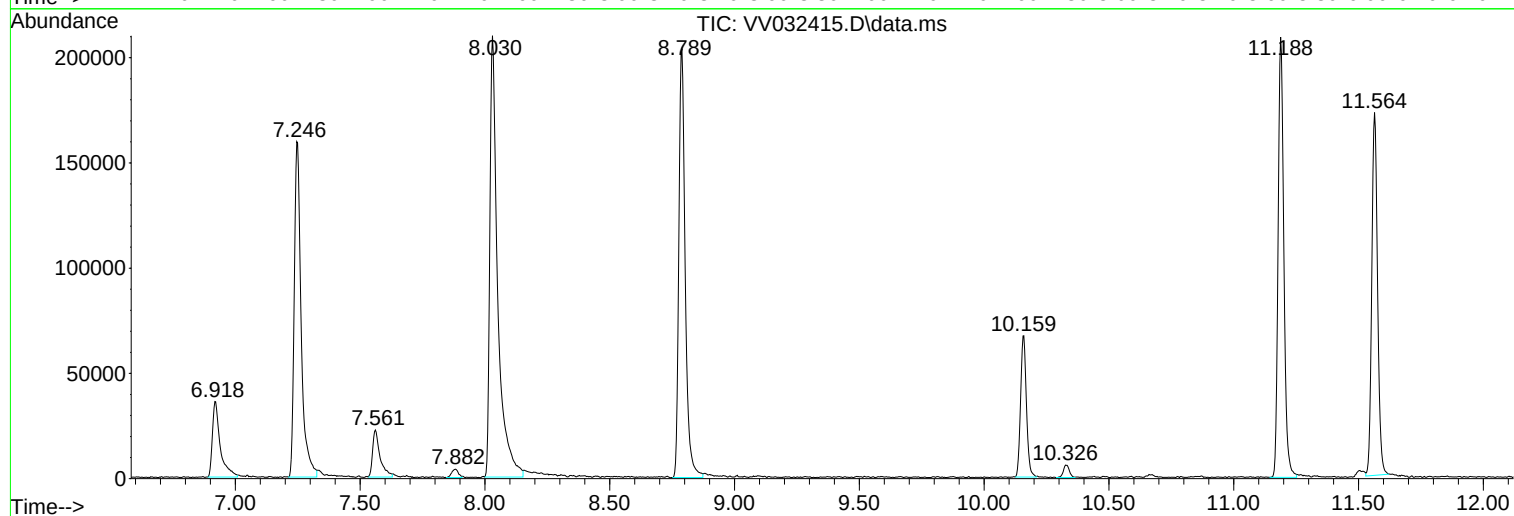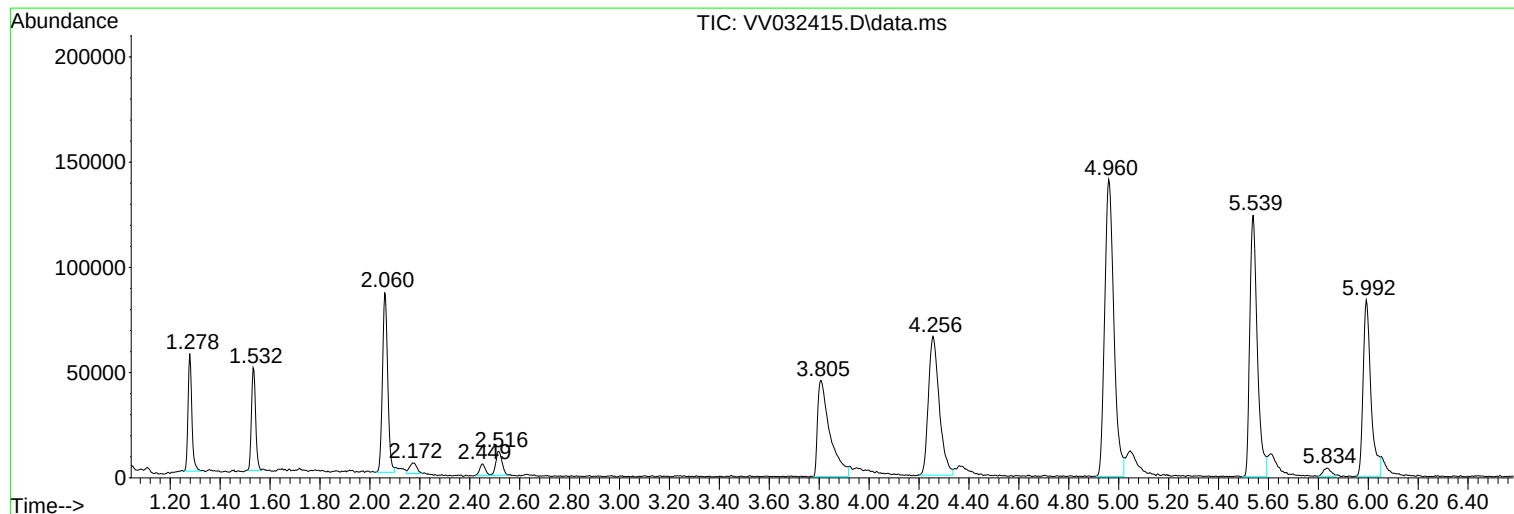

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032415.D
Acq On : 12 Oct 2023 14:34
Operator : SY/MD
Sample : 04851-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032415.D
Acq On : 12 Oct 2023 14:34
Operator : SY/MD
Sample : 04851-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc