

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
 Data File : VV032418.D
 Acq On : 12 Oct 2023 15:46
 Operator : SY/MD
 Sample : 04851-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B06

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032418.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	16	21	29	rVB	4801	6458	1.49%	0.200%
2	1.278	67	74	84	rBV	51021	54453	12.60%	1.683%
3	1.532	147	153	168	rVB	45854	53767	12.44%	1.662%
4	2.060	306	317	334	rBV	78896	118483	27.41%	3.663%
5	3.812	852	862	897	rBV	42473	150453	34.81%	4.651%
6	4.252	983	999	1022	rBV2	58106	156127	36.12%	4.827%
7	4.963	1203	1220	1240	rBV3	129417	336361	77.82%	10.399%
8	5.539	1389	1399	1415	rBV	113194	240372	55.61%	7.431%
9	5.995	1529	1541	1580	rBV	76679	184789	42.75%	5.713%
10	6.921	1817	1829	1860	rBV	33015	75472	17.46%	2.333%
11	7.249	1917	1931	1951	rBV	145393	281366	65.10%	8.699%
12	7.561	2019	2028	2044	rBV2	19796	40009	9.26%	1.237%
13	7.908	2119	2136	2156	rVB3	22707	50525	11.69%	1.562%
14	8.030	2165	2174	2206	rBV	203096	432227	100.00%	13.363%
15	8.188	2214	2223	2237	rVB7	6970	15140	3.50%	0.468%
16	8.789	2399	2410	2430	rBV	195057	335914	77.72%	10.385%
17	10.159	2822	2836	2854	rBV	65393	107611	24.90%	3.327%
18	10.329	2880	2889	2901	rBV2	8123	13521	3.13%	0.418%
19	11.188	3145	3156	3179	rBV	197250	314618	72.79%	9.727%
20	11.564	3256	3273	3292	rBV	163801	261880	60.59%	8.096%
21	12.201	3460	3471	3477	rBV4	3048	5032	1.16%	0.156%




Sum of corrected areas: 3234578

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032418.D
Acq On : 12 Oct 2023 15:46
Operator : SY/MD
Sample : 04851-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

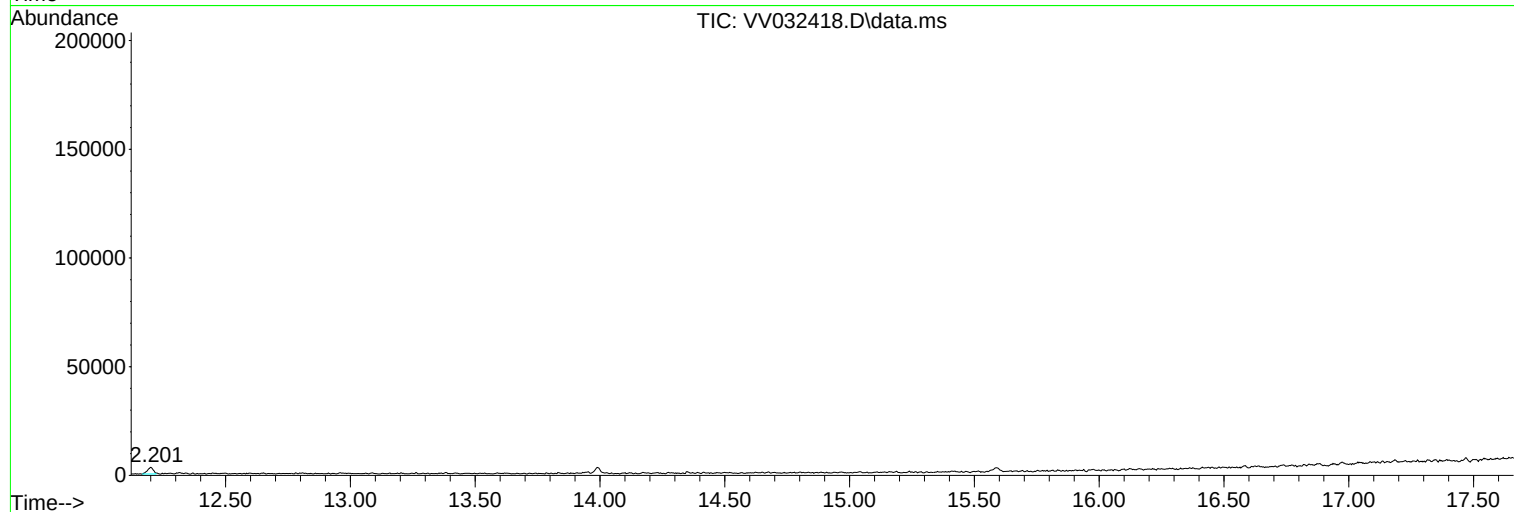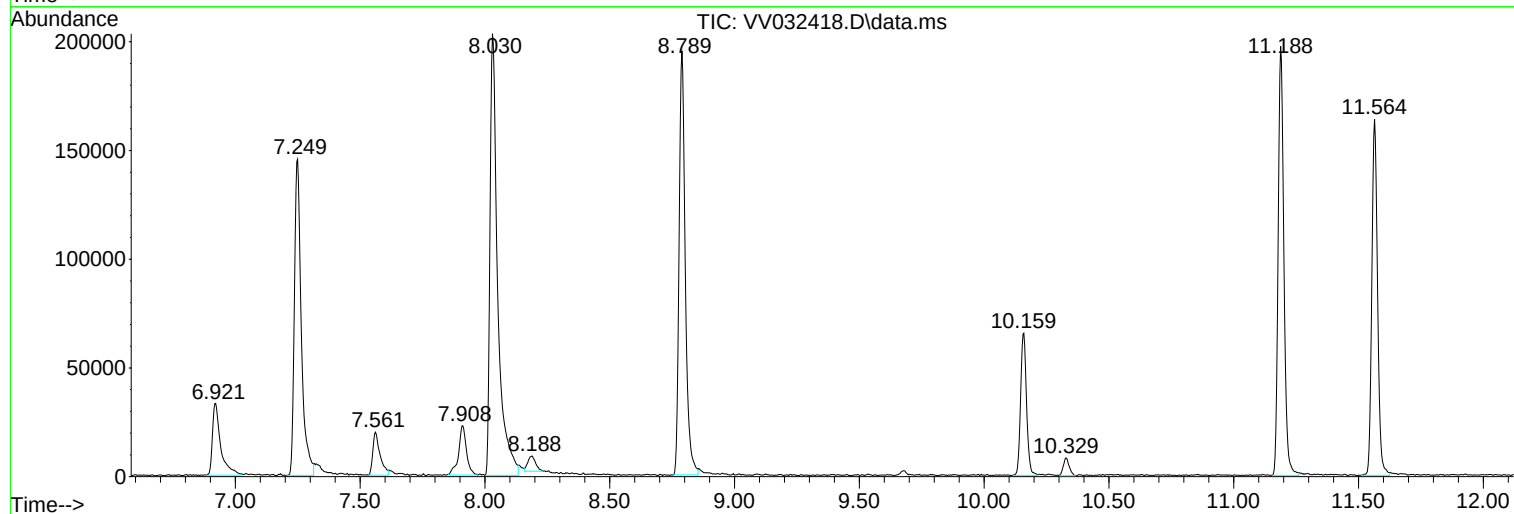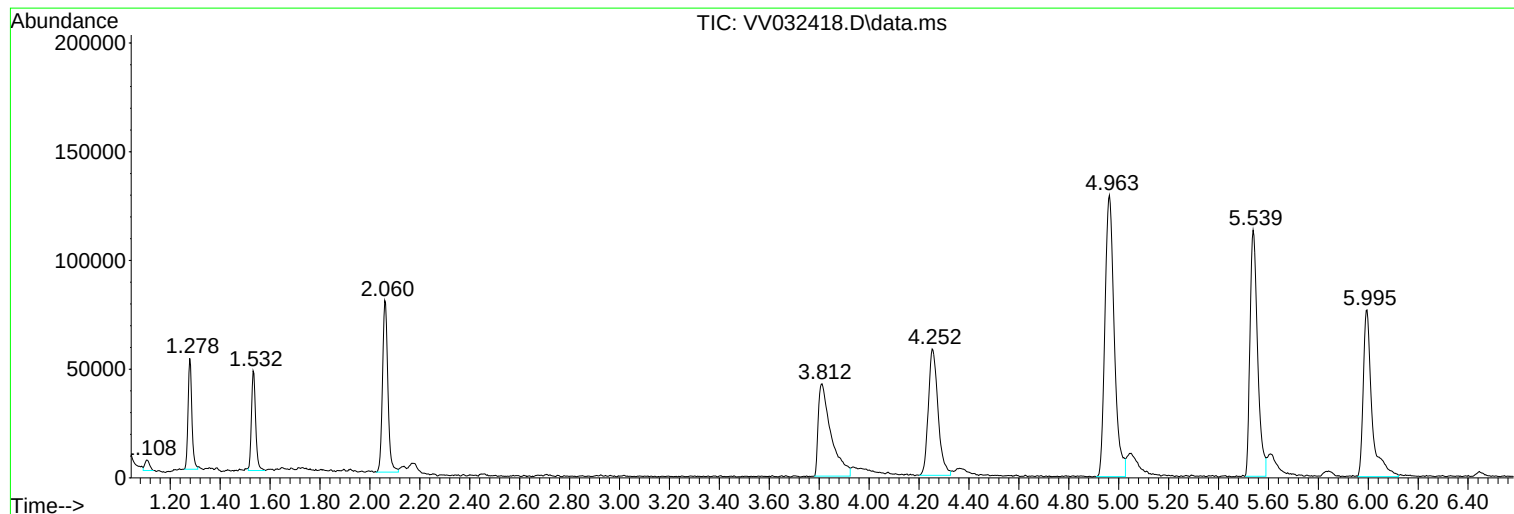

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032418.D
Acq On : 12 Oct 2023 15:46
Operator : SY/MD
Sample : 04851-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032418.D
Acq On : 12 Oct 2023 15:46
Operator : SY/MD
Sample : 04851-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B06

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------