


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101223\
Data File : VV032406.D
Acq On : 12 Oct 2023 08:34
Operator : SY/MD
Sample : BFB220
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB220

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Oct 12 22:36:28 2023

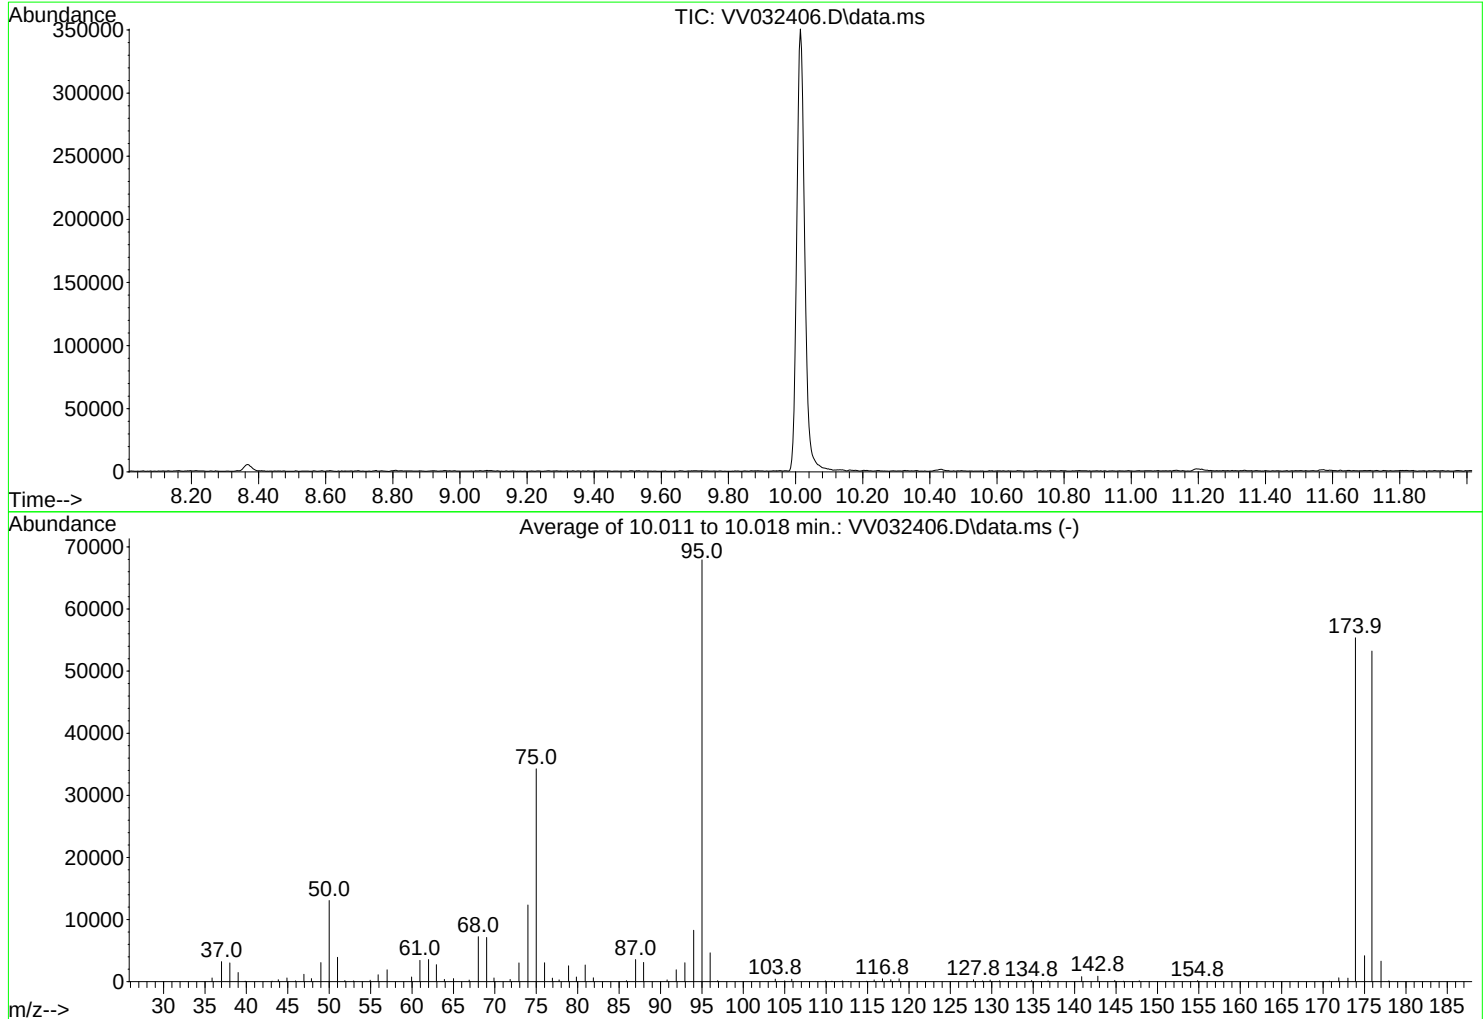

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	13073	PASS
75	95	30	80	50.4	34264	PASS
95	95	100	100	100.0	67923	PASS
96	95	5	9	6.8	4645	PASS
173	174	0.00	2	1.1	582	PASS
174	95	50	120	81.5	55373	PASS
175	174	5	9	7.5	4168	PASS
176	174	95	105	96.1	53221	PASS
177	176	5	10	6.2	3290	PASS

m/z	Abundance
35.90	114.0
37.00	140.0
39.80	246.0
43.90	350.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

m/z	Abundance
35.90	698.0
37.00	3342.0
38.00	3111.0
39.00	1470.0
39.90	340.0
43.90	617.0
44.90	614.0
45.90	115.0
46.90	1149.0
47.90	483.0
49.00	3193.0
50.00	13075.0
51.00	3947.0
51.90	183.0
53.00	168.0
54.90	241.0
55.90	1059.0
57.00	1915.0
60.00	769.0
60.90	3544.0
62.00	3446.0
63.00	2703.0
63.90	359.0
65.00	511.0
66.90	254.0
68.00	7186.0
69.00	7159.0
69.90	626.0
71.80	318.0
72.90	2992.0
74.00	12471.0
75.00	34192.0
76.00	3071.0
77.00	514.0
77.70	281.0
78.90	2649.0
79.90	734.0
80.90	2768.0
81.90	658.0
85.90	170.0
87.00	3515.0
87.90	3004.0
90.80	298.0
91.90	1987.0
93.00	3013.0
94.00	8208.0
95.00	66656.0
96.00	4671.0
96.90	152.0
103.90	458.0
104.90	119.0
105.90	432.0
109.90	131.0
110.70	130.0
111.90	125.0
115.80	272.0
116.80	486.0
117.80	313.0
118.80	468.0
127.90	311.0
129.00	123.0
129.80	284.0
130.90	159.0
134.80	167.0
136.90	125.0
140.90	810.0
142.80	883.0
144.90	214.0
147.80	160.0
154.80	175.0
170.70	106.0
171.90	563.0
173.00	838.0
173.90	53336.0
175.00	4096.0
175.90	50552.0
177.00	3263.0
178.00	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

m/z	Abundance
35.90	739.0
37.00	3487.0
38.00	3145.0
39.00	1530.0
39.90	324.0
43.10	119.0
43.80	653.0
44.90	610.0
46.00	135.0
47.00	1227.0
47.90	500.0
49.00	3166.0
50.00	13430.0
51.00	4058.0
51.90	191.0
53.00	136.0
55.00	230.0
55.90	1150.0
57.00	2000.0
59.90	764.0
61.00	3521.0
62.00	3702.0
62.90	2829.0
63.90	371.0
65.00	500.0
66.90	259.0
68.00	7484.0
69.00	7362.0
69.90	603.0
71.80	371.0
72.90	3050.0
74.00	12768.0
75.00	35344.0
76.00	3122.0
76.90	571.0
77.80	299.0
78.90	2598.0
79.80	780.0
80.90	2758.0
81.90	656.0
85.90	166.0
87.00	3733.0
88.00	3178.0
90.80	289.0
91.90	1951.0
92.90	3134.0
94.00	8542.0
95.00	70104.0
96.00	4776.0
96.90	162.0
103.90	446.0
105.00	153.0
105.80	428.0
109.90	134.0
110.70	118.0
111.90	139.0
114.90	112.0
115.80	292.0
116.80	500.0
117.80	296.0
118.80	485.0
127.80	317.0
128.90	125.0
129.80	271.0
131.00	154.0
134.80	180.0
135.90	102.0
136.80	133.0
140.80	834.0
142.80	898.0
144.80	205.0
145.90	126.0
147.80	180.0
154.90	191.0
170.80	109.0
171.90	638.0
173.00	907.0
173.90	57136.0
175.00	4296.0
175.90	54760.0
177.00	3381.0
178.00	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

m/z	Abundance
35.90	712.0
37.00	3283.0
38.00	2832.0
39.00	1428.0
39.90	301.0
43.10	122.0
43.90	681.0
44.90	562.0
46.00	132.0
47.00	1164.0
47.80	506.0
49.00	2808.0
50.00	12714.0
51.00	3784.0
51.90	204.0
52.80	101.0
54.90	222.0
55.90	1123.0
57.00	1837.0
59.90	696.0
61.00	3261.0
62.00	3531.0
62.90	2659.0
63.90	361.0
65.00	469.0
66.90	234.0
68.00	7075.0
69.00	6845.0
69.90	535.0
71.90	409.0
72.90	2982.0
74.00	11773.0
75.00	33256.0
76.00	2951.0
76.90	630.0
77.80	304.0
78.90	2413.0
79.80	766.0
80.90	2481.0
81.90	582.0
85.90	165.0
87.00	3432.0
88.00	3137.0
90.80	262.0
91.90	1823.0
93.00	3005.0
94.00	8054.0
95.00	67008.0
96.00	4488.0
96.90	145.0
103.80	334.0
105.10	156.0
105.90	340.0
109.90	117.0
112.00	120.0
112.70	112.0
114.90	121.0
115.80	263.0
116.80	449.0
117.80	297.0
118.80	466.0
127.70	332.0
128.80	152.0
129.80	240.0
131.00	124.0
134.80	198.0
136.70	133.0
140.80	788.0
142.80	829.0
144.90	183.0
145.90	126.0
147.80	172.0
154.90	189.0
161.00	105.0
171.90	644.0
173.90	55648.0
175.00	4113.0
175.90	54352.0
177.00	3227.0
177.90	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220