

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101320\
 Data File : VV018872.D
 Acq On : 13 Oct 2020 12:56
 Operator : SY/MD
 Sample : L4308-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW1

Quant Time: Oct 14 20:38:57 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 14 01:28:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	355651	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	349934	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	164757	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	130219	40.30	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.60%
7) Chloroethane-d5	1.58	69	104448	40.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.30%
11) 1,1-Dichloroethene-d2	2.12	63	193071	30.99	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.98%
21) 2-Butanone-d5	3.91	46	184511	92.99	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.99%
24) Chloroform-d	4.38	84	238014	41.75	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.50%
26) 1,2-Dichloroethane-d4	5.06	65	167896	43.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.88%
32) Benzene-d6	5.08	84	484824	43.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.10%
36) 1,2-Dichloropropane-d6	6.09	67	156615	42.65	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.30%
41) Toluene-d8	7.34	98	423155	42.33	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.66%
43) trans-1,3-Dichloropropene-	7.64	79	72140	40.19	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.38%
47) 2-Hexanone-d5	8.11	63	100184	77.84	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	77.84%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	157032	37.17	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	74.34%
64) 1,2-Dichlorobenzene-d4	11.65	152	172579	47.33	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.66%


Target Compounds					Ovalue
13) Acetone	2.19	43	16052	9.706 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101320\
Data File : VV018872.D
Acq On : 13 Oct 2020 12:56
Operator : SY/MD
Sample : L4308-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW1

Quant Time: Oct 14 20:38:57 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 14 01:28:12 2020
Response via : Initial Calibration

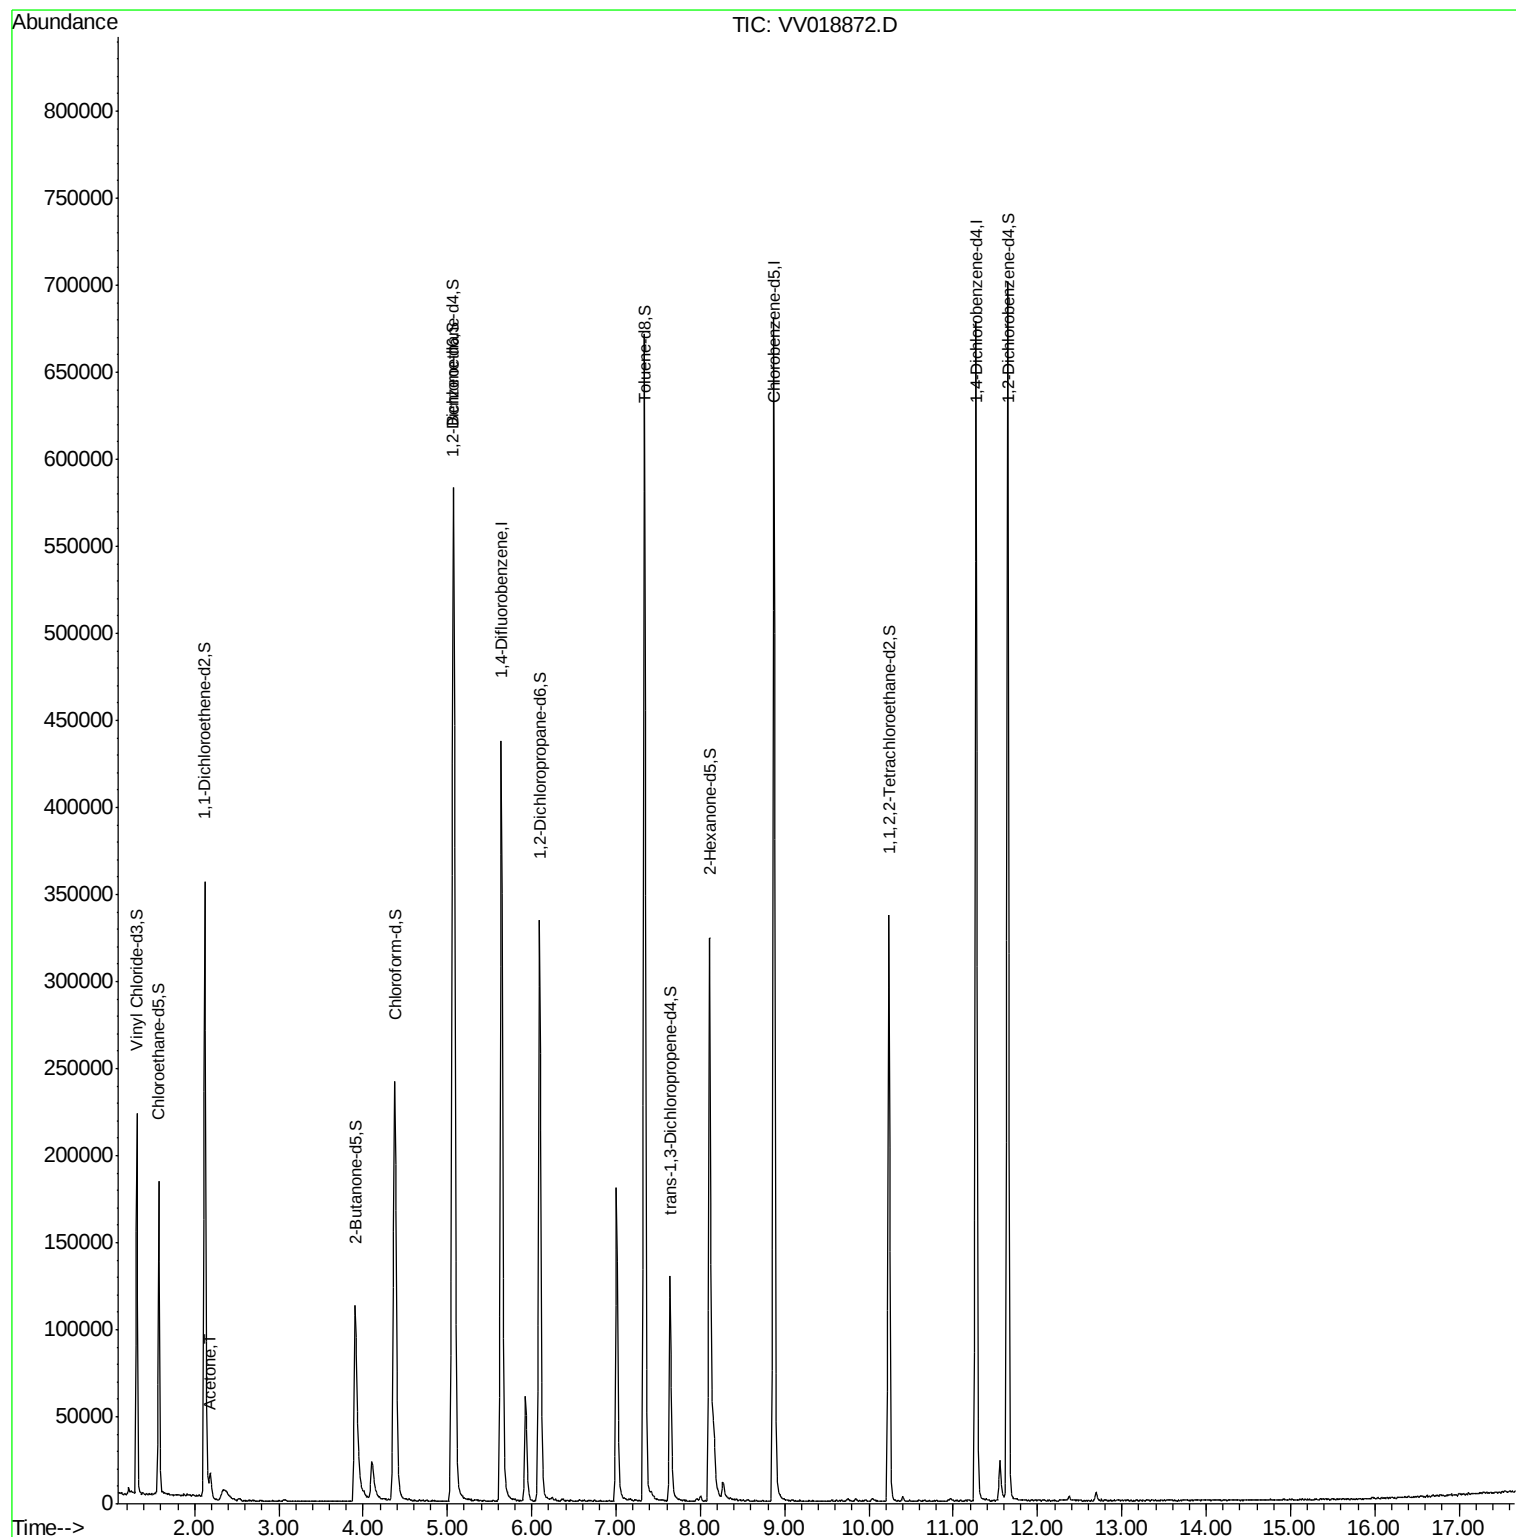

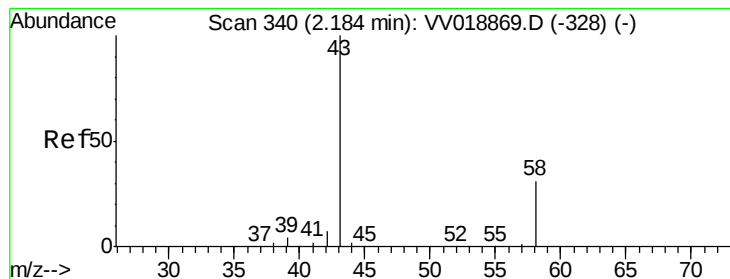

#13

Acetone

Concen: 9.706 ug/L

RT: 2.19 min Scan# 341

Delta R.T. 0.00 min

Lab File: VV018872.D

Acq: 13 Oct 2020 12:56

Instrument :
MSVOA_V
ClientSampleId :
C0AW1

Tot Ion: 43 Resp: 16052

Ion Ratio Lower Upper

43 100

58 33.5 0.0 61.0

