

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101320\
 Data File : VV018874.D
 Acq On : 13 Oct 2020 13:44
 Operator : SY/MD
 Sample : L4351-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	84	rVB	205687	208731	14.47%	1.938%
2	1.576	144	151	164	rBV	172971	189001	13.10%	1.755%
3	2.119	311	320	352	rVB	340995	525918	36.46%	4.882%
4	2.495	434	437	439	rBV3	495	305	0.02%	0.003%
5	2.862	547	551	555	rBV	295	284	0.02%	0.003%
6	2.881	555	557	561	rVV	387	286	0.02%	0.003%
7	2.913	565	567	569	rBV	265	161	0.01%	0.001%
8	3.003	594	595	596	rBV	196	54	0.00%	0.001%
9	3.055	609	611	612	rBV	396	186	0.01%	0.002%
10	3.225	661	664	669	rVB3	537	403	0.03%	0.004%
11	3.351	697	703	705	rBV	370	307	0.02%	0.003%
12	3.386	711	714	715	rBV2	217	132	0.01%	0.001%
13	3.415	721	723	725	rBV	301	158	0.01%	0.001%
14	3.428	725	727	728	rVV	312	125	0.01%	0.001%
15	3.438	728	730	732	rVB3	555	217	0.02%	0.002%
16	3.457	733	736	738	rBV	293	185	0.01%	0.002%
17	3.518	750	755	761	rBV2	543	579	0.04%	0.005%
18	3.582	770	775	778	rBV2	354	424	0.03%	0.004%
19	3.614	783	785	788	rVB2	529	241	0.02%	0.002%
20	3.637	790	792	798	rVB2	319	215	0.01%	0.002%
21	3.676	802	804	805	rBV2	258	98	0.01%	0.001%
22	3.714	814	816	817	rBV	343	127	0.01%	0.001%
23	3.907	865	876	913	rBV	105872	303276	21.02%	2.815%
24	4.373	1007	1021	1050	rVB	223343	555239	38.49%	5.155%
25	4.595	1086	1090	1094	rBV3	544	479	0.03%	0.004%
26	4.733	1131	1133	1135	rVB	264	102	0.01%	0.001%
27	4.775	1144	1146	1147	rBV	130	33	0.00%	0.000%
28	4.785	1147	1149	1152	rBV2	417	241	0.02%	0.002%
29	4.859	1168	1172	1173	rBV	278	177	0.01%	0.002%
30	4.868	1173	1175	1181	rVV4	433	432	0.03%	0.004%
31	4.936	1193	1196	1200	rBV2	424	408	0.03%	0.004%
32	5.071	1219	1238	1269	rBV2	565516	1442570	100.00%	13.392%
33	5.322	1314	1316	1317	rBV	426	149	0.01%	0.001%
34	5.486	1366	1367	1369	rVB2	319	96	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101320\
 Data File : VV018874.D
 Acq On : 13 Oct 2020 13:44
 Operator : SY/MD
 Sample : L4351-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

35	5.499	1369	1371	1373	rBV3	502	215	0.01%	0.002%
36	5.531	1380	1381	1383	rVB	225	75	0.01%	0.001%
37	5.566	1391	1392	1395	rVB	358	150	0.01%	0.001%
38	5.582	1395	1397	1400	rBV3	627	364	0.03%	0.003%
39	5.640	1403	1415	1442	rBV	423003	841887	58.36%	7.816%
40	5.926	1493	1504	1528	rVB	58991	121026	8.39%	1.124%
41	6.093	1538	1556	1578	rBV	325767	661620	45.86%	6.142%
42	6.322	1624	1627	1629	rBV	628	385	0.03%	0.004%
43	6.415	1654	1656	1657	rVB	319	96	0.01%	0.001%
44	6.431	1657	1661	1664	rBV3	440	392	0.03%	0.004%
45	6.463	1669	1671	1672	rBV	460	163	0.01%	0.002%
46	6.566	1700	1703	1708	rBV2	328	332	0.02%	0.003%
47	6.656	1729	1731	1733	rBV	194	108	0.01%	0.001%
48	6.672	1733	1736	1739	rVV	438	252	0.02%	0.002%
49	6.685	1739	1740	1744	rVB3	358	217	0.02%	0.002%
50	6.769	1761	1766	1768	rBV3	411	327	0.02%	0.003%
51	6.781	1768	1770	1773	rVV2	417	201	0.01%	0.002%
52	6.801	1774	1776	1778	rVB	452	194	0.01%	0.002%
53	6.814	1778	1780	1782	rBV2	247	119	0.01%	0.001%
54	6.827	1782	1784	1791	rVV3	434	364	0.03%	0.003%
55	6.923	1811	1814	1816	rBV2	433	227	0.02%	0.002%
56	6.955	1822	1824	1825	rBV2	199	79	0.01%	0.001%
57	6.965	1825	1827	1829	rVV	413	170	0.01%	0.002%
58	7.007	1829	1840	1870	rVV	171708	317246	21.99%	2.945%
59	7.338	1931	1943	1963	rBV	647839	1110964	77.01%	10.314%
60	7.643	2027	2038	2065	rBV	128019	221572	15.36%	2.057%
61	7.923	2122	2125	2128	rBV2	398	317	0.02%	0.003%
62	8.003	2143	2150	2158	rVB7	2458	3487	0.24%	0.032%
63	8.106	2172	2182	2221	rBV2	308639	666189	46.18%	6.185%
64	8.669	2354	2357	2363	rBV4	585	690	0.05%	0.006%
65	8.797	2394	2397	2398	rBV2	486	157	0.01%	0.001%
66	8.871	2408	2420	2453	rBV	655189	1065427	73.86%	9.891%
67	9.135	2500	2502	2504	rBV2	557	215	0.01%	0.002%
68	9.167	2510	2512	2515	rBV3	422	237	0.02%	0.002%
69	9.222	2527	2529	2530	rBV	393	137	0.01%	0.001%
70	9.293	2549	2551	2553	rBV	316	177	0.01%	0.002%
71	9.312	2554	2557	2560	rVB3	655	411	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101320\
 Data File : VV018874.D
 Acq On : 13 Oct 2020 13:44
 Operator : SY/MD
 Sample : L4351-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

72	9.566	2634	2636	2638	rVB3	278	112	0.01%	0.001%
73	9.598	2644	2646	2649	rBV2	664	324	0.02%	0.003%
74	9.701	2674	2678	2681	rBV2	421	446	0.03%	0.004%
75	9.855	2724	2726	2728	rBV	349	183	0.01%	0.002%
76	9.929	2745	2749	2750	rBV2	374	286	0.02%	0.003%
77	10.238	2830	2845	2865	rBV	321276	505287	35.03%	4.691%
78	10.331	2871	2874	2877	rBV2	404	298	0.02%	0.003%
79	10.633	2966	2968	2974	rVB2	318	234	0.02%	0.002%
80	10.662	2974	2977	2980	rBV2	372	314	0.02%	0.003%
81	10.707	2988	2991	2992	rBV2	287	175	0.01%	0.002%
82	10.945	3060	3065	3070	rVB2	545	565	0.04%	0.005%
83	11.270	3154	3166	3187	rBV	635493	974833	67.58%	9.050%
84	11.511	3239	3241	3244	rBV	531	328	0.02%	0.003%
85	11.569	3249	3259	3265	rVV5	1519	2684	0.19%	0.025%
86	11.646	3271	3283	3307	rBV	653597	1026474	71.16%	9.529%
87	12.135	3432	3435	3440	rVB2	532	380	0.03%	0.004%
88	12.756	3624	3628	3633	rVB5	2114	2217	0.15%	0.021%
89	12.981	3691	3698	3714	rVB4	5387	8328	0.58%	0.077%
90	13.379	3819	3822	3828	rBV2	687	741	0.05%	0.007%


Sum of corrected areas: 10771737

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101320\
Data File : VV018874.D
Acq On : 13 Oct 2020 13:44
Operator : SY/MD
Sample : L4351-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

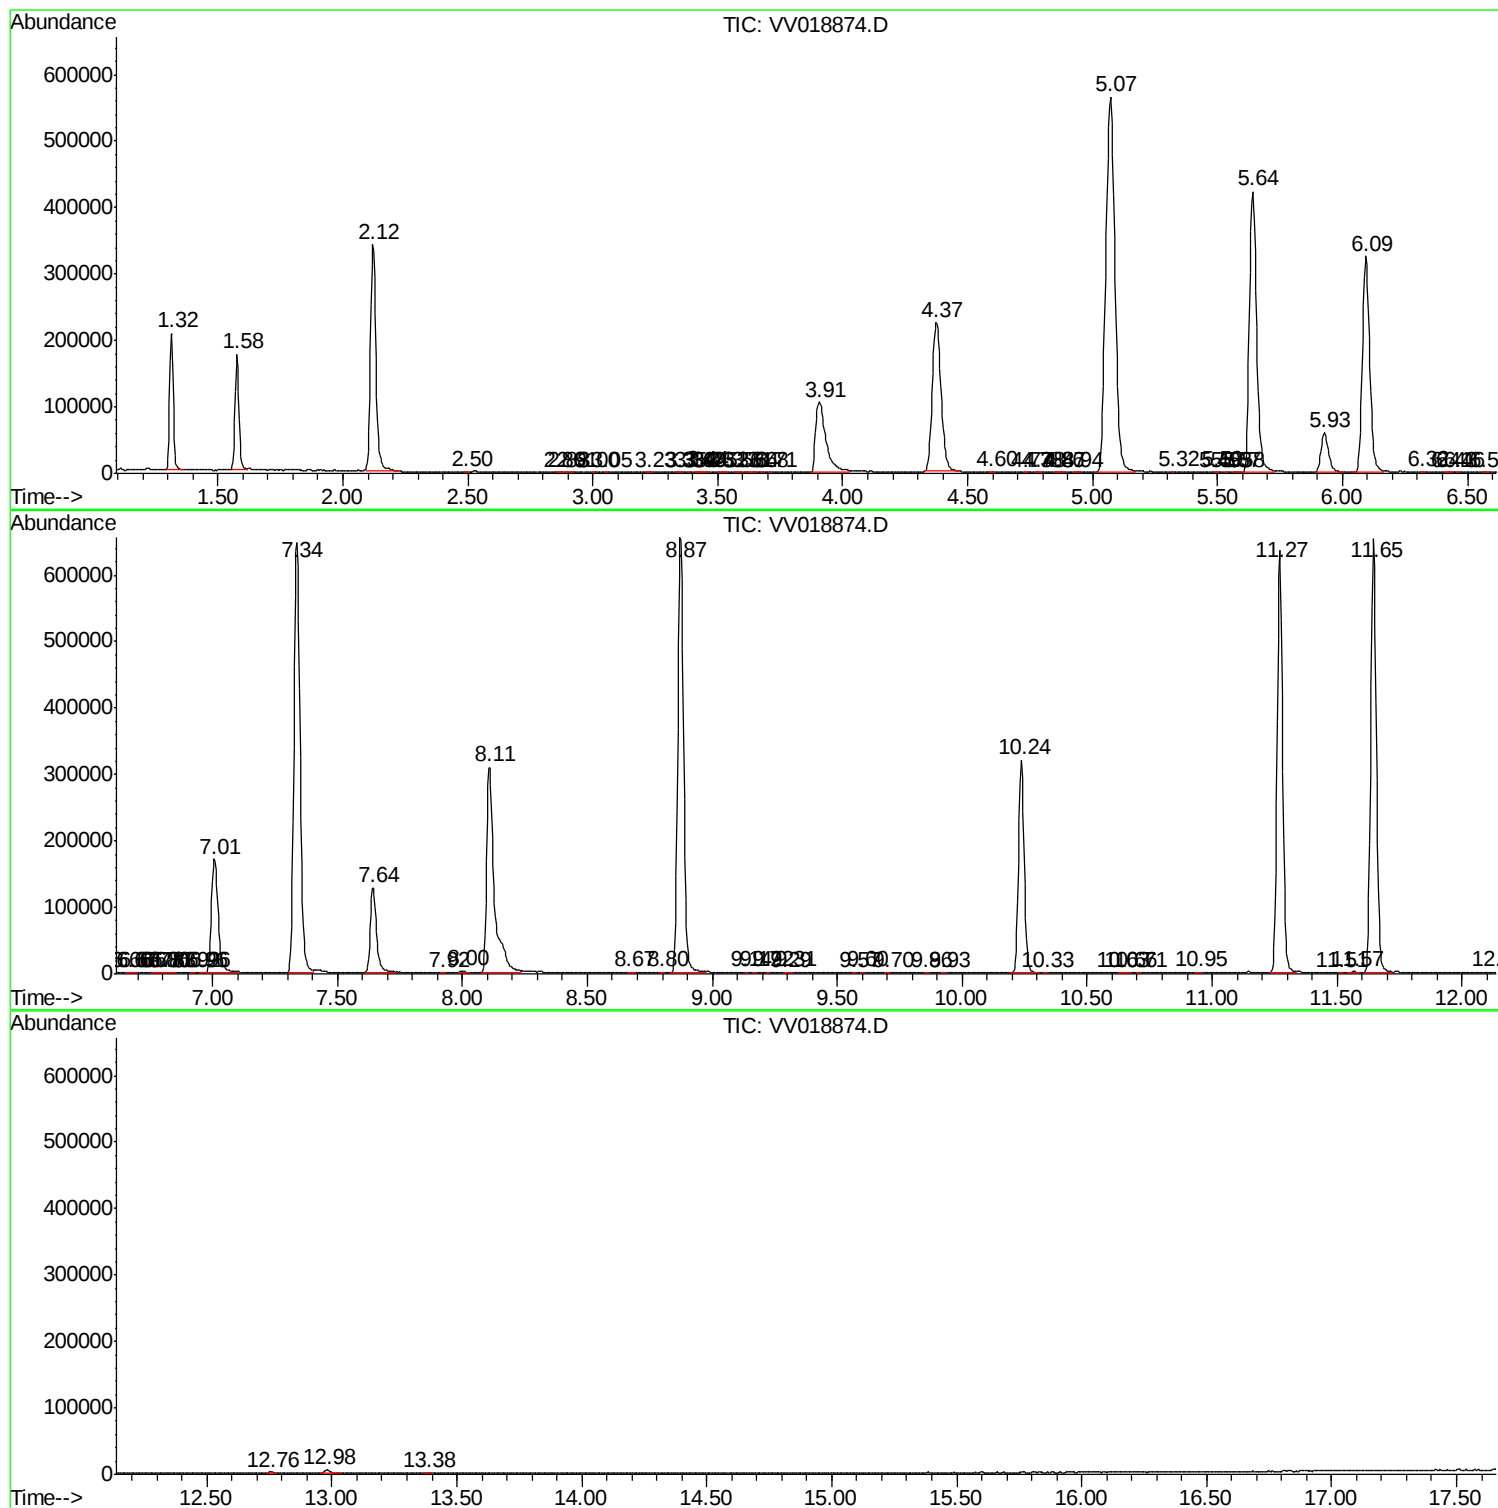

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101320\
Data File : VV018874.D
Acq On : 13 Oct 2020 13:44
Operator : SY/MD
Sample : L4351-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV101320\
Data File : VV018874.D
Acq On : 13 Oct 2020 13:44
Operator : SY/MD
Sample : L4351-06
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AL3

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
