

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101320\
 Data File : VV018882.D
 Acq On : 13 Oct 2020 17:02
 Operator : SY/MD
 Sample : L4351-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	84	rVB2	237997	249770	17.61%	2.191%
2	1.579	144	152	169	rBV	168244	188860	13.31%	1.657%
3	2.122	311	321	349	rVB	335160	521151	36.74%	4.572%
4	2.563	456	458	461	rVB	264	112	0.01%	0.001%
5	2.605	469	471	472	rBV	460	196	0.01%	0.002%
6	2.714	502	505	508	rBV	255	172	0.01%	0.002%
7	2.778	521	525	538	rVB7	2625	4772	0.34%	0.042%
8	2.856	546	549	551	rBV3	261	217	0.02%	0.002%
9	2.920	567	569	573	rVB2	406	212	0.01%	0.002%
10	3.071	612	616	618	rBV2	671	407	0.03%	0.004%
11	3.203	653	657	662	rBV2	520	569	0.04%	0.005%
12	3.270	676	678	680	rBV	188	93	0.01%	0.001%
13	3.293	680	685	687	rBV3	375	271	0.02%	0.002%
14	3.376	707	711	717	rVB4	418	410	0.03%	0.004%
15	3.434	727	729	731	rBV	125	75	0.01%	0.001%
16	3.454	731	735	737	rBV2	366	260	0.02%	0.002%
17	3.576	771	773	776	rBV2	104	61	0.00%	0.001%
18	3.595	776	779	782	rBV2	334	260	0.02%	0.002%
19	3.621	785	787	790	rVB	356	193	0.01%	0.002%
20	3.653	793	797	799	rBV	358	231	0.02%	0.002%
21	3.695	807	810	812	rBV2	298	137	0.01%	0.001%
22	3.724	815	819	825	rVB2	486	465	0.03%	0.004%
23	3.759	825	830	831	rBV	313	258	0.02%	0.002%
24	3.798	837	842	845	rBV2	447	284	0.02%	0.002%
25	3.830	851	852	856	rBB2	266	120	0.01%	0.001%
26	3.868	860	864	866	rBV2	391	281	0.02%	0.002%
27	3.933	866	884	917	rBV3	308310	942552	66.44%	8.269%
28	4.373	1006	1021	1055	rBV	221491	553179	38.99%	4.853%
29	4.621	1094	1098	1103	rBV5	525	533	0.04%	0.005%
30	4.656	1107	1109	1115	rVB3	445	328	0.02%	0.003%
31	4.733	1130	1133	1138	rVB3	449	351	0.02%	0.003%
32	4.756	1138	1140	1141	rBV	315	129	0.01%	0.001%
33	4.849	1167	1169	1173	rVB3	380	218	0.02%	0.002%
34	4.881	1176	1179	1182	rBV3	404	272	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101320\
 Data File : VV018882.D
 Acq On : 13 Oct 2020 17:02
 Operator : SY/MD
 Sample : L4351-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

35	4.958	1197	1203	1204	rBV2	478	325	0.02%	0.003%
36	4.994	1213	1214	1215	rBV2	229	81	0.01%	0.001%
37	5.071	1220	1238	1270	rBV2	551783	1418601	100.00%	12.446%
38	5.280	1301	1303	1305	rBV3	571	317	0.02%	0.003%
39	5.354	1322	1326	1328	rBV2	520	514	0.04%	0.005%
40	5.486	1363	1367	1369	rBV4	293	216	0.02%	0.002%
41	5.499	1369	1371	1374	rVB2	545	294	0.02%	0.003%
42	5.569	1391	1393	1395	rBV	273	124	0.01%	0.001%
43	5.640	1403	1415	1445	rBV	425143	848120	59.79%	7.441%
44	5.926	1493	1504	1524	rBV	40709	86532	6.10%	0.759%
45	6.093	1541	1556	1585	rBV	317843	648155	45.69%	5.686%
46	6.402	1647	1652	1654	rBV2	430	363	0.03%	0.003%
47	6.450	1665	1667	1669	rVB2	366	148	0.01%	0.001%
48	6.463	1669	1671	1672	rBV	192	76	0.01%	0.001%
49	6.473	1672	1674	1677	rBV	337	161	0.01%	0.001%
50	6.662	1730	1733	1734	rBV	458	230	0.02%	0.002%
51	6.762	1762	1764	1766	rBV	308	171	0.01%	0.002%
52	6.878	1796	1800	1803	rBV	249	246	0.02%	0.002%
53	6.916	1810	1812	1813	rBV	391	154	0.01%	0.001%
54	7.007	1829	1840	1864	rBV	171064	311640	21.97%	2.734%
55	7.238	1909	1912	1913	rBV3	743	453	0.03%	0.004%
56	7.334	1930	1942	1967	rBV	634093	1087906	76.69%	9.544%
57	7.640	2026	2037	2059	rBV	121487	213291	15.04%	1.871%
58	7.884	2108	2113	2116	rBV2	527	553	0.04%	0.005%
59	7.990	2139	2146	2149	rBV6	1657	1808	0.13%	0.016%
60	8.061	2167	2168	2169	rBV6	222	72	0.01%	0.001%
61	8.106	2172	2182	2226	rVV2	318209	657191	46.33%	5.766%
62	8.511	2306	2308	2310	rBV	379	206	0.01%	0.002%
63	8.624	2341	2343	2345	rBV2	555	249	0.02%	0.002%
64	8.678	2358	2360	2361	rBV	410	206	0.01%	0.002%
65	8.704	2366	2368	2371	rBV	387	202	0.01%	0.002%
66	8.772	2386	2389	2392	rVB4	356	221	0.02%	0.002%
67	8.871	2408	2420	2446	rBV	666150	1071898	75.56%	9.404%
68	9.222	2528	2529	2532	rBV	125	75	0.01%	0.001%
69	9.257	2538	2540	2545	rBV2	343	279	0.02%	0.002%
70	9.431	2591	2594	2597	rBV2	385	173	0.01%	0.002%
71	9.460	2601	2603	2605	rBV	320	146	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101320\
 Data File : VV018882.D
 Acq On : 13 Oct 2020 17:02
 Operator : SY/MD
 Sample : L4351-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

72	9.576	2636	2639	2641	rBV	268	174	0.01%	0.002%
73	9.646	2657	2661	2663	rBV2	448	335	0.02%	0.003%
74	9.691	2672	2675	2678	rBV	272	154	0.01%	0.001%
75	9.855	2723	2726	2729	rVB2	351	209	0.01%	0.002%
76	10.016	2774	2776	2777	rVB	295	76	0.01%	0.001%
77	10.026	2777	2779	2781	rBV	341	154	0.01%	0.001%
78	10.235	2833	2844	2873	rVB	349606	548875	38.69%	4.815%
79	10.334	2873	2875	2879	rBV2	341	241	0.02%	0.002%
80	10.415	2898	2900	2904	rVB3	503	334	0.02%	0.003%
81	10.685	2982	2984	2988	rVB2	416	251	0.02%	0.002%
82	10.714	2989	2993	2997	rBV2	403	396	0.03%	0.003%
83	10.765	3007	3009	3013	rBV2	346	255	0.02%	0.002%
84	10.804	3013	3021	3022	rBV3	403	460	0.03%	0.004%
85	11.125	3115	3121	3124	rBV3	413	453	0.03%	0.004%
86	11.270	3154	3166	3187	rBV	662096	996092	70.22%	8.739%
87	11.399	3202	3206	3211	rBV4	1033	966	0.07%	0.008%
88	11.530	3246	3247	3250	rBV2	439	223	0.02%	0.002%
89	11.646	3271	3283	3305	rBV	657189	1027029	72.40%	9.010%
90	11.865	3348	3351	3354	rBV2	638	443	0.03%	0.004%
91	12.112	3421	3428	3433	rVB4	618	839	0.06%	0.007%
92	12.138	3433	3436	3438	rBV2	368	240	0.02%	0.002%
93	12.228	3461	3464	3468	rBV2	471	403	0.03%	0.004%
94	13.116	3738	3740	3744	rBV3	503	429	0.03%	0.004%
95	13.447	3837	3843	3845	rBV4	452	440	0.03%	0.004%


Sum of corrected areas: 11398267

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101320\
Data File : VV018882.D
Acq On : 13 Oct 2020 17:02
Operator : SY/MD
Sample : L4351-03DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

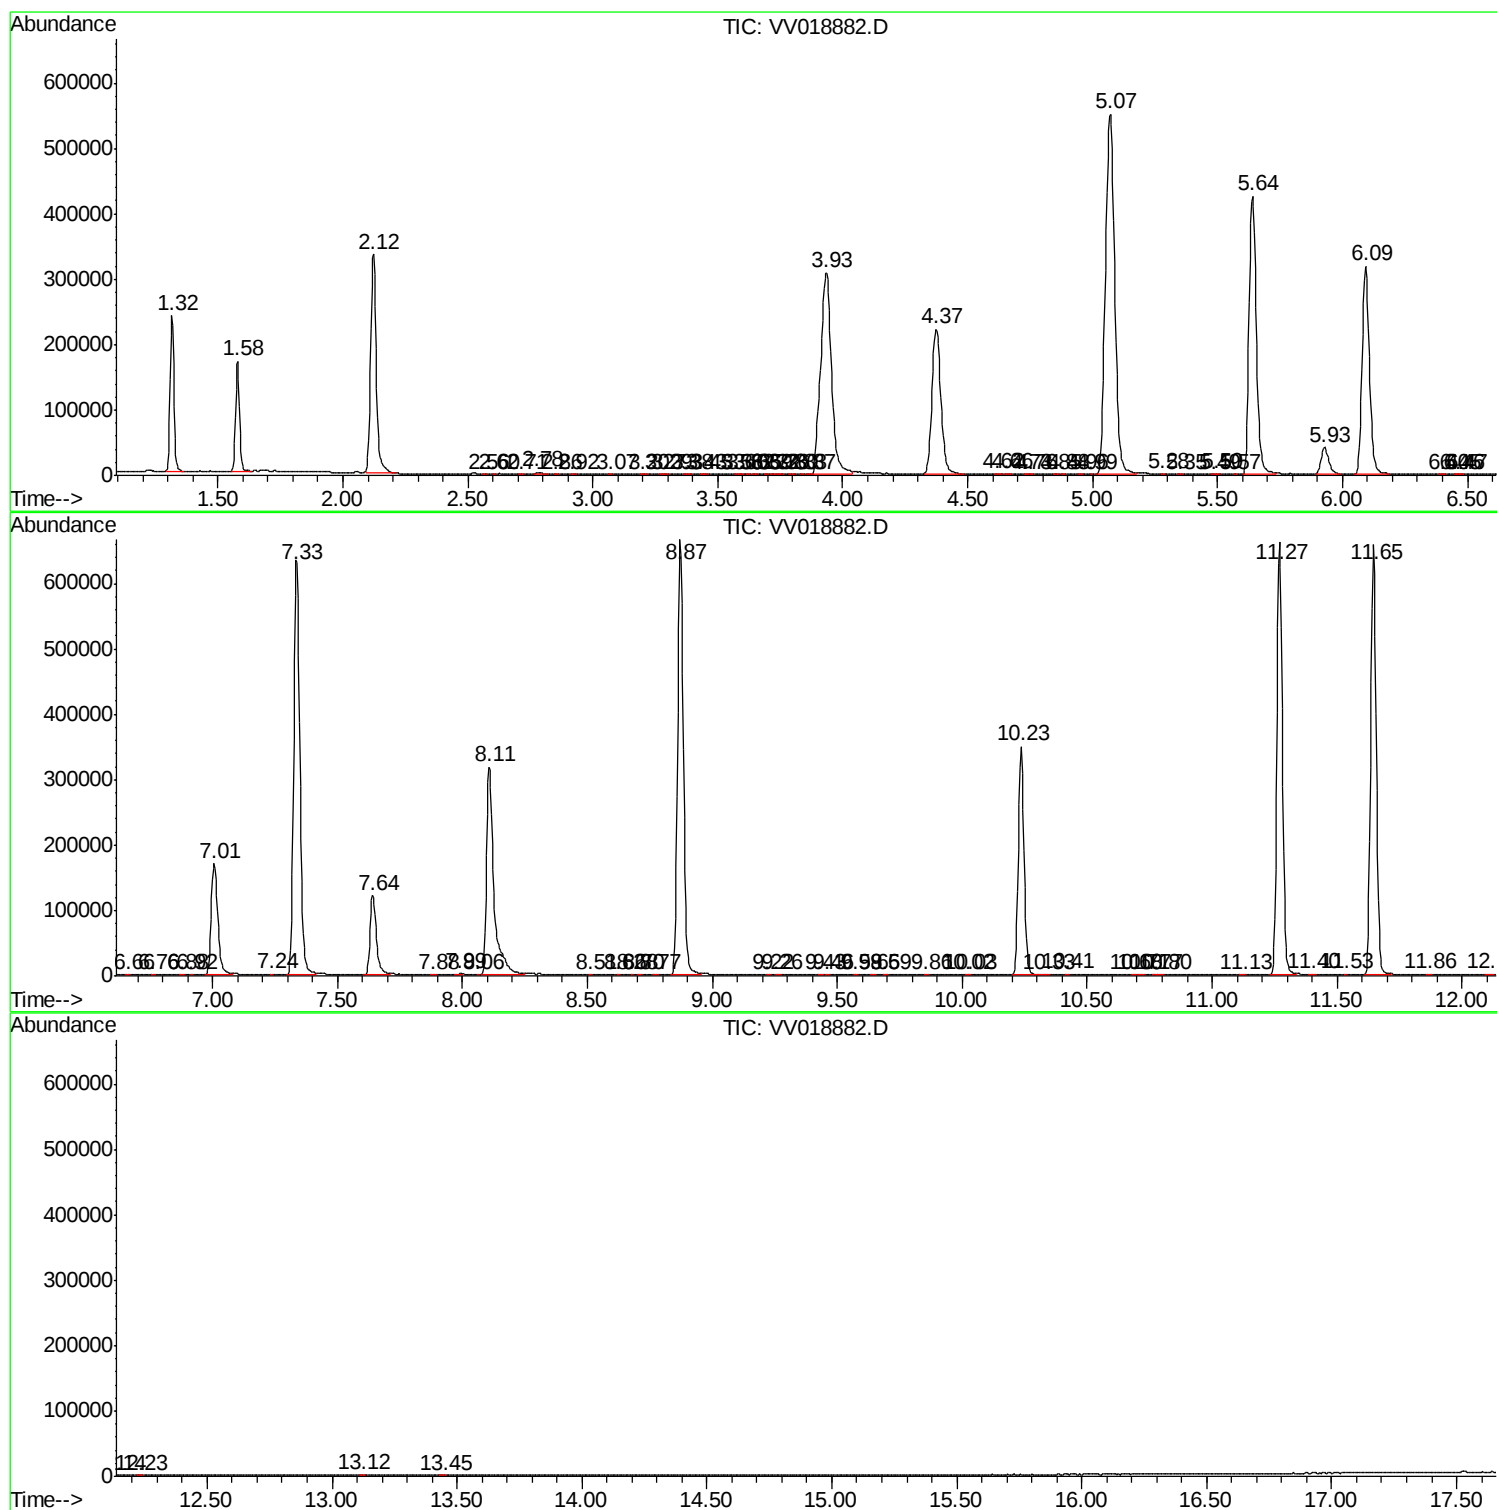

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101320\
Data File : VV018882.D
Acq On : 13 Oct 2020 17:02
Operator : SY/MD
Sample : L4351-03DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV101320\
Data File : VV018882.D
Acq On : 13 Oct 2020 17:02
Operator : SY/MD
Sample : L4351-03DL 10X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AH9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc