

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101320\
 Data File : VV018884.D
 Acq On : 13 Oct 2020 18:13
 Operator : SY/MD
 Sample : VIBLK64
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK64

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	82	rVB	194327	192377	13.77%	1.827%
2	1.576	144	151	169	rBV	165486	188085	13.46%	1.786%
3	2.122	311	321	349	rVB	324560	497658	35.61%	4.725%
4	2.592	464	467	469	rBV	452	253	0.02%	0.002%
5	2.621	473	476	478	rBV2	564	421	0.03%	0.004%
6	2.881	556	557	558	rBV	287	86	0.01%	0.001%
7	3.000	592	594	598	rVB2	443	253	0.02%	0.002%
8	3.064	610	614	622	rVB7	762	913	0.07%	0.009%
9	3.235	665	667	669	rBV	94	51	0.00%	0.000%
10	3.257	669	674	678	rVV2	300	313	0.02%	0.003%
11	3.444	730	732	738	rBV	344	312	0.02%	0.003%
12	3.486	743	745	746	rBV	234	109	0.01%	0.001%
13	3.531	757	759	761	rBV2	333	157	0.01%	0.001%
14	3.579	771	774	776	rBV	476	327	0.02%	0.003%
15	3.752	822	828	829	rBV2	430	380	0.03%	0.004%
16	3.820	847	849	854	rVB2	532	423	0.03%	0.004%
17	3.846	854	857	861	rBV2	390	382	0.03%	0.004%
18	3.868	861	864	866	rBV2	314	233	0.02%	0.002%
19	3.910	866	877	905	rBV	102645	303815	21.74%	2.885%
20	4.376	1004	1022	1048	rBV	222964	552737	39.55%	5.248%
21	4.685	1116	1118	1121	rBV	464	284	0.02%	0.003%
22	4.723	1128	1130	1132	rBV2	442	213	0.02%	0.002%
23	4.820	1156	1160	1161	rBV2	380	249	0.02%	0.002%
24	4.900	1181	1185	1188	rBV2	327	260	0.02%	0.002%
25	4.949	1194	1200	1203	rBV3	565	667	0.05%	0.006%
26	5.003	1214	1217	1221	rVB2	471	431	0.03%	0.004%
27	5.071	1221	1238	1270	rBV2	541756	1397500	100.00%	13.269%
28	5.373	1329	1332	1335	rBV3	283	227	0.02%	0.002%
29	5.437	1349	1352	1354	rBV3	482	325	0.02%	0.003%
30	5.518	1375	1377	1378	rBV3	357	170	0.01%	0.002%
31	5.640	1403	1415	1443	rBV	416572	836791	59.88%	7.945%
32	5.929	1493	1505	1523	rBV	43582	92554	6.62%	0.879%
33	6.045	1537	1541	1543	rBV	320	249	0.02%	0.002%
34	6.093	1543	1556	1587	rBV	320488	649413	46.47%	6.166%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101320\
 Data File : VV018884.D
 Acq On : 13 Oct 2020 18:13
 Operator : SY/MD
 Sample : VIBLK64
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK64

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

35	6.341	1632	1633	1635	rBV	325	157	0.01%	0.001%
36	6.395	1647	1650	1654	rBV	471	273	0.02%	0.003%
37	6.421	1654	1658	1664	rBV4	456	511	0.04%	0.005%
38	6.479	1673	1676	1678	rBV	368	179	0.01%	0.002%
39	6.540	1692	1695	1699	rVB2	646	368	0.03%	0.003%
40	6.598	1712	1713	1716	rVB2	359	168	0.01%	0.002%
41	6.649	1727	1729	1730	rBV	318	108	0.01%	0.001%
42	6.871	1795	1798	1801	rBV2	522	346	0.02%	0.003%
43	6.923	1812	1814	1817	rBV2	380	229	0.02%	0.002%
44	7.006	1828	1840	1863	rBV	164091	299406	21.42%	2.843%
45	7.338	1931	1943	1975	rBV	625336	1072971	76.78%	10.188%
46	7.592	2019	2022	2024	rBV2	545	356	0.03%	0.003%
47	7.643	2028	2038	2060	rVV	119235	208538	14.92%	1.980%
48	8.003	2144	2150	2156	rBV5	1587	2190	0.16%	0.021%
49	8.109	2173	2183	2225	rBV2	307840	638184	45.67%	6.059%
50	8.688	2361	2363	2367	rBV2	463	301	0.02%	0.003%
51	8.871	2409	2420	2441	rBV	663931	1069466	76.53%	10.154%
52	9.235	2531	2533	2534	rBV	296	94	0.01%	0.001%
53	9.376	2575	2577	2581	rBV2	357	320	0.02%	0.003%
54	9.550	2628	2631	2634	rVB2	532	342	0.02%	0.003%
55	9.855	2724	2726	2727	rBV2	355	150	0.01%	0.001%
56	9.926	2745	2748	2753	rBV2	517	444	0.03%	0.004%
57	10.183	2826	2828	2830	rBV	417	235	0.02%	0.002%
58	10.238	2833	2845	2862	rVV	339585	533936	38.21%	5.070%
59	10.730	2995	2998	3002	rBV	462	414	0.03%	0.004%
60	10.855	3033	3037	3040	rBV3	550	446	0.03%	0.004%
61	11.270	3154	3166	3194	rBV	637607	978960	70.05%	9.295%
62	11.646	3271	3283	3308	rBV	640502	1003227	71.79%	9.526%
63	12.070	3413	3415	3420	rVB	559	349	0.02%	0.003%
64	13.742	3933	3935	3936	rBV	529	244	0.02%	0.002%
65	13.778	3941	3946	3947	rBV	531	433	0.03%	0.004%


Sum of corrected areas: 10531963

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101320\
Data File : VV018884.D
Acq On : 13 Oct 2020 18:13
Operator : SY/MD
Sample : VIBLK64
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK64

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

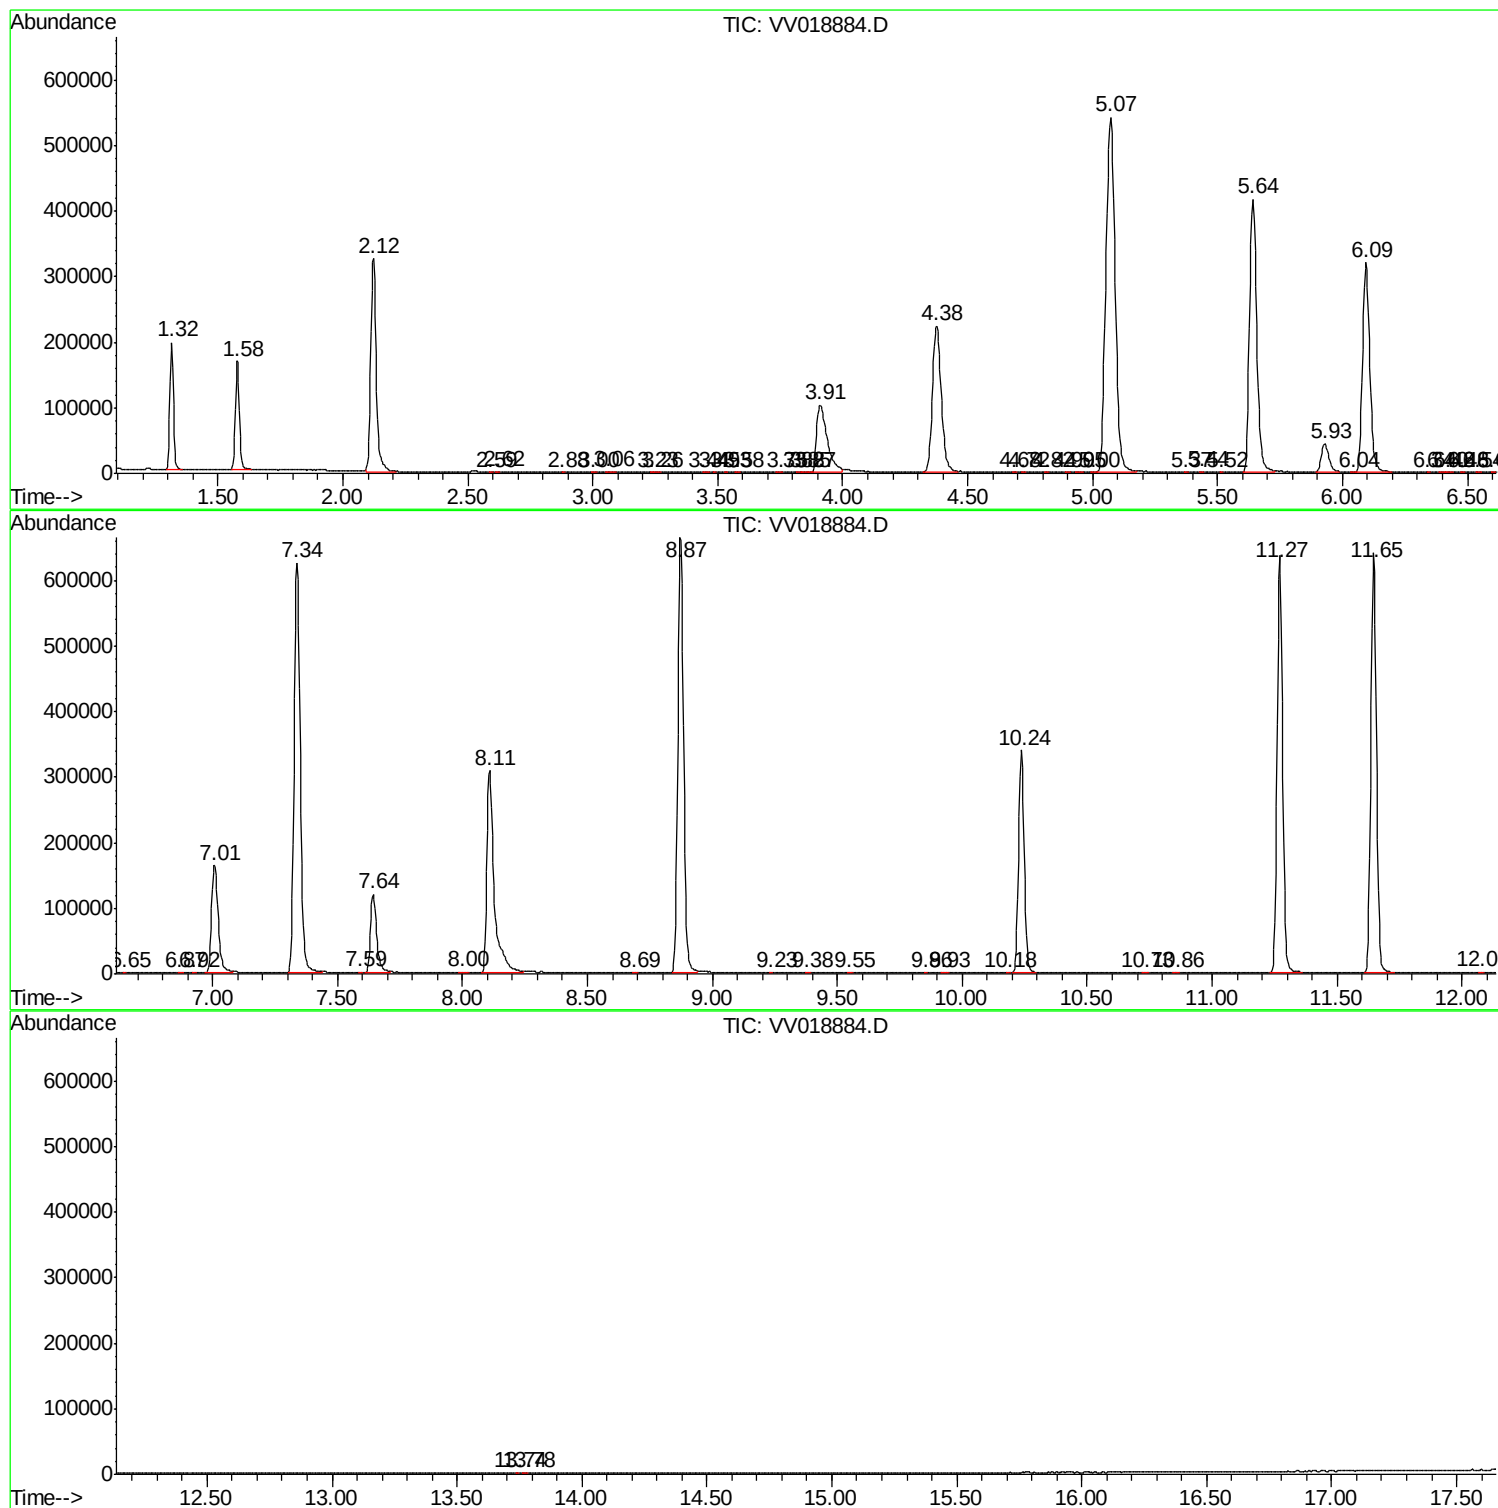

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101320\
Data File : VV018884.D
Acq On : 13 Oct 2020 18:13
Operator : SY/MD
Sample : VIBLK64
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK64

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV101320\
Data File : VV018884.D
Acq On : 13 Oct 2020 18:13
Operator : SY/MD
Sample : VIBLK64
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK64

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc