

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101320\
 Data File : VV018886.D
 Acq On : 13 Oct 2020 19:00
 Operator : SY/MD
 Sample : L4351-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	63	70	87	rVB2	214563	224527	10.50%	1.693%
2	1.576	144	151	166	rVB	165742	184934	8.65%	1.394%
3	2.119	311	320	347	rVB2	328400	522441	24.42%	3.939%
4	2.598	466	469	473	rBV2	488	333	0.02%	0.003%
5	2.631	477	479	484	rVB2	508	323	0.02%	0.002%
6	2.727	507	509	511	rBV3	408	148	0.01%	0.001%
7	2.782	516	526	541	rBV4	19567	39192	1.83%	0.296%
8	2.946	576	577	581	rVB	397	193	0.01%	0.001%
9	3.020	599	600	603	rVB2	258	102	0.00%	0.001%
10	3.049	604	609	610	rBV	610	427	0.02%	0.003%
11	3.094	622	623	626	rBV	127	76	0.00%	0.001%
12	3.123	629	632	634	rBV	445	251	0.01%	0.002%
13	3.187	650	652	656	rBV2	245	215	0.01%	0.002%
14	3.348	700	702	705	rBV2	294	136	0.01%	0.001%
15	3.460	735	737	738	rBV2	127	42	0.00%	0.000%
16	3.512	747	753	757	rBV4	651	731	0.03%	0.006%
17	3.605	778	782	784	rBV2	449	316	0.01%	0.002%
18	3.618	784	786	787	rBV2	298	147	0.01%	0.001%
19	3.659	798	799	801	rBV	241	131	0.01%	0.001%
20	3.688	805	808	810	rBV2	284	200	0.01%	0.002%
21	3.733	819	822	826	rVB	246	167	0.01%	0.001%
22	3.753	826	828	832	rBV	342	256	0.01%	0.002%
23	3.775	832	835	836	rBV	306	179	0.01%	0.001%
24	3.865	862	863	865	rVB	386	122	0.01%	0.001%
25	3.936	865	885	925	rBV2	783571	2139162	100.00%	16.129%
26	4.377	1006	1022	1051	rBV	218782	544817	25.47%	4.108%
27	4.698	1118	1122	1126	rBV2	512	435	0.02%	0.003%
28	4.872	1173	1176	1178	rBV	298	205	0.01%	0.002%
29	4.981	1206	1210	1213	rVB3	499	419	0.02%	0.003%
30	5.010	1217	1219	1221	rBV2	300	135	0.01%	0.001%
31	5.071	1221	1238	1268	rBV2	542266	1393322	65.13%	10.506%
32	5.563	1387	1391	1395	rBV4	696	651	0.03%	0.005%
33	5.640	1403	1415	1444	rBV	409198	819539	38.31%	6.179%
34	5.936	1492	1507	1538	rBV3	469403	954116	44.60%	7.194%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101320\
 Data File : VV018886.D
 Acq On : 13 Oct 2020 19:00
 Operator : SY/MD
 Sample : L4351-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

35	6.093	1543	1556	1581	rVV	314814	636386	29.75%	4.798%
36	6.383	1644	1646	1647	rBV	355	131	0.01%	0.001%
37	6.598	1710	1713	1715	rVB2	422	223	0.01%	0.002%
38	6.611	1715	1717	1719	rBV	354	151	0.01%	0.001%
39	6.666	1732	1734	1736	rBV2	262	94	0.00%	0.001%
40	6.743	1756	1758	1761	rVB2	416	198	0.01%	0.001%
41	6.769	1763	1766	1772	rVB2	513	534	0.02%	0.004%
42	6.798	1772	1775	1779	rBV2	438	348	0.02%	0.003%
43	6.827	1781	1784	1788	rVV3	261	187	0.01%	0.001%
44	6.852	1790	1792	1795	rVV2	519	218	0.01%	0.002%
45	6.907	1805	1809	1811	rBV3	344	209	0.01%	0.002%
46	6.926	1811	1815	1818	rVB2	586	462	0.02%	0.003%
47	6.946	1818	1821	1823	rBV	374	236	0.01%	0.002%
48	7.007	1829	1840	1867	rBV	166883	303322	14.18%	2.287%
49	7.338	1931	1943	1963	rBV	609562	1065659	49.82%	8.035%
50	7.643	2026	2038	2056	rBV	119101	210848	9.86%	1.590%
51	7.933	2125	2128	2131	rBV2	312	233	0.01%	0.002%
52	8.000	2139	2149	2162	rVB2	22590	39727	1.86%	0.300%
53	8.106	2172	2182	2218	rBV2	324857	661816	30.94%	4.990%
54	8.624	2341	2343	2344	rBV	260	149	0.01%	0.001%
55	8.701	2364	2367	2370	rVB3	598	347	0.02%	0.003%
56	8.746	2376	2381	2382	rBV3	452	329	0.02%	0.002%
57	8.871	2408	2420	2443	rBV	635004	1028709	48.09%	7.756%
58	9.135	2500	2502	2504	rBV	439	210	0.01%	0.002%
59	9.331	2561	2563	2564	rBV	381	152	0.01%	0.001%
60	9.396	2580	2583	2586	rBV	470	254	0.01%	0.002%
61	9.415	2587	2589	2591	rBV	303	137	0.01%	0.001%
62	9.428	2591	2593	2594	rBV	289	111	0.01%	0.001%
63	9.466	2602	2605	2608	rVB2	445	225	0.01%	0.002%
64	9.650	2660	2662	2663	rBV2	521	207	0.01%	0.002%
65	9.675	2667	2670	2674	rBV3	401	381	0.02%	0.003%
66	9.762	2696	2697	2700	rVB2	372	122	0.01%	0.001%
67	9.814	2711	2713	2717	rVB2	419	273	0.01%	0.002%
68	9.833	2717	2719	2721	rBV2	240	121	0.01%	0.001%
69	9.891	2734	2737	2740	rVB2	388	243	0.01%	0.002%
70	9.910	2741	2743	2745	rBV	398	158	0.01%	0.001%
71	10.100	2800	2802	2803	rBV	314	98	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV101320\
 Data File : VV018886.D
 Acq On : 13 Oct 2020 19:00
 Operator : SY/MD
 Sample : L4351-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis

72	10.238	2830	2845	2870	rBV	353816	551620	25.79%	4.159%
73	10.379	2882	2889	2890	rBV4	745	792	0.04%	0.006%
74	10.560	2941	2945	2948	rBV2	437	283	0.01%	0.002%
75	10.714	2990	2993	2995	rBV2	317	211	0.01%	0.002%
76	10.878	3042	3044	3047	rBV	415	230	0.01%	0.002%
77	10.994	3075	3080	3086	rBV3	460	594	0.03%	0.004%
78	11.029	3086	3091	3093	rBV2	557	488	0.02%	0.004%
79	11.122	3114	3120	3123	rBV2	922	869	0.04%	0.007%
80	11.270	3154	3166	3189	rBV	608616	931358	43.54%	7.022%
81	11.508	3237	3240	3242	rBV	557	391	0.02%	0.003%
82	11.646	3271	3283	3309	rBV	635980	991064	46.33%	7.473%
83	11.868	3350	3352	3354	rBV	435	210	0.01%	0.002%
84	12.322	3490	3493	3496	rBV3	470	343	0.02%	0.003%
85	12.350	3500	3502	3503	rBV	268	87	0.00%	0.001%
86	12.820	3645	3648	3652	rBV2	542	524	0.02%	0.004%
87	13.051	3719	3720	3722	rBV2	340	169	0.01%	0.001%
88	13.412	3830	3832	3839	rVB2	451	384	0.02%	0.003%
89	14.151	4052	4062	4066	rBV3	765	1414	0.07%	0.011%


Sum of corrected areas: 13262629

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV101320\
Data File : VV018886.D
Acq On : 13 Oct 2020 19:00
Operator : SY/MD
Sample : L4351-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

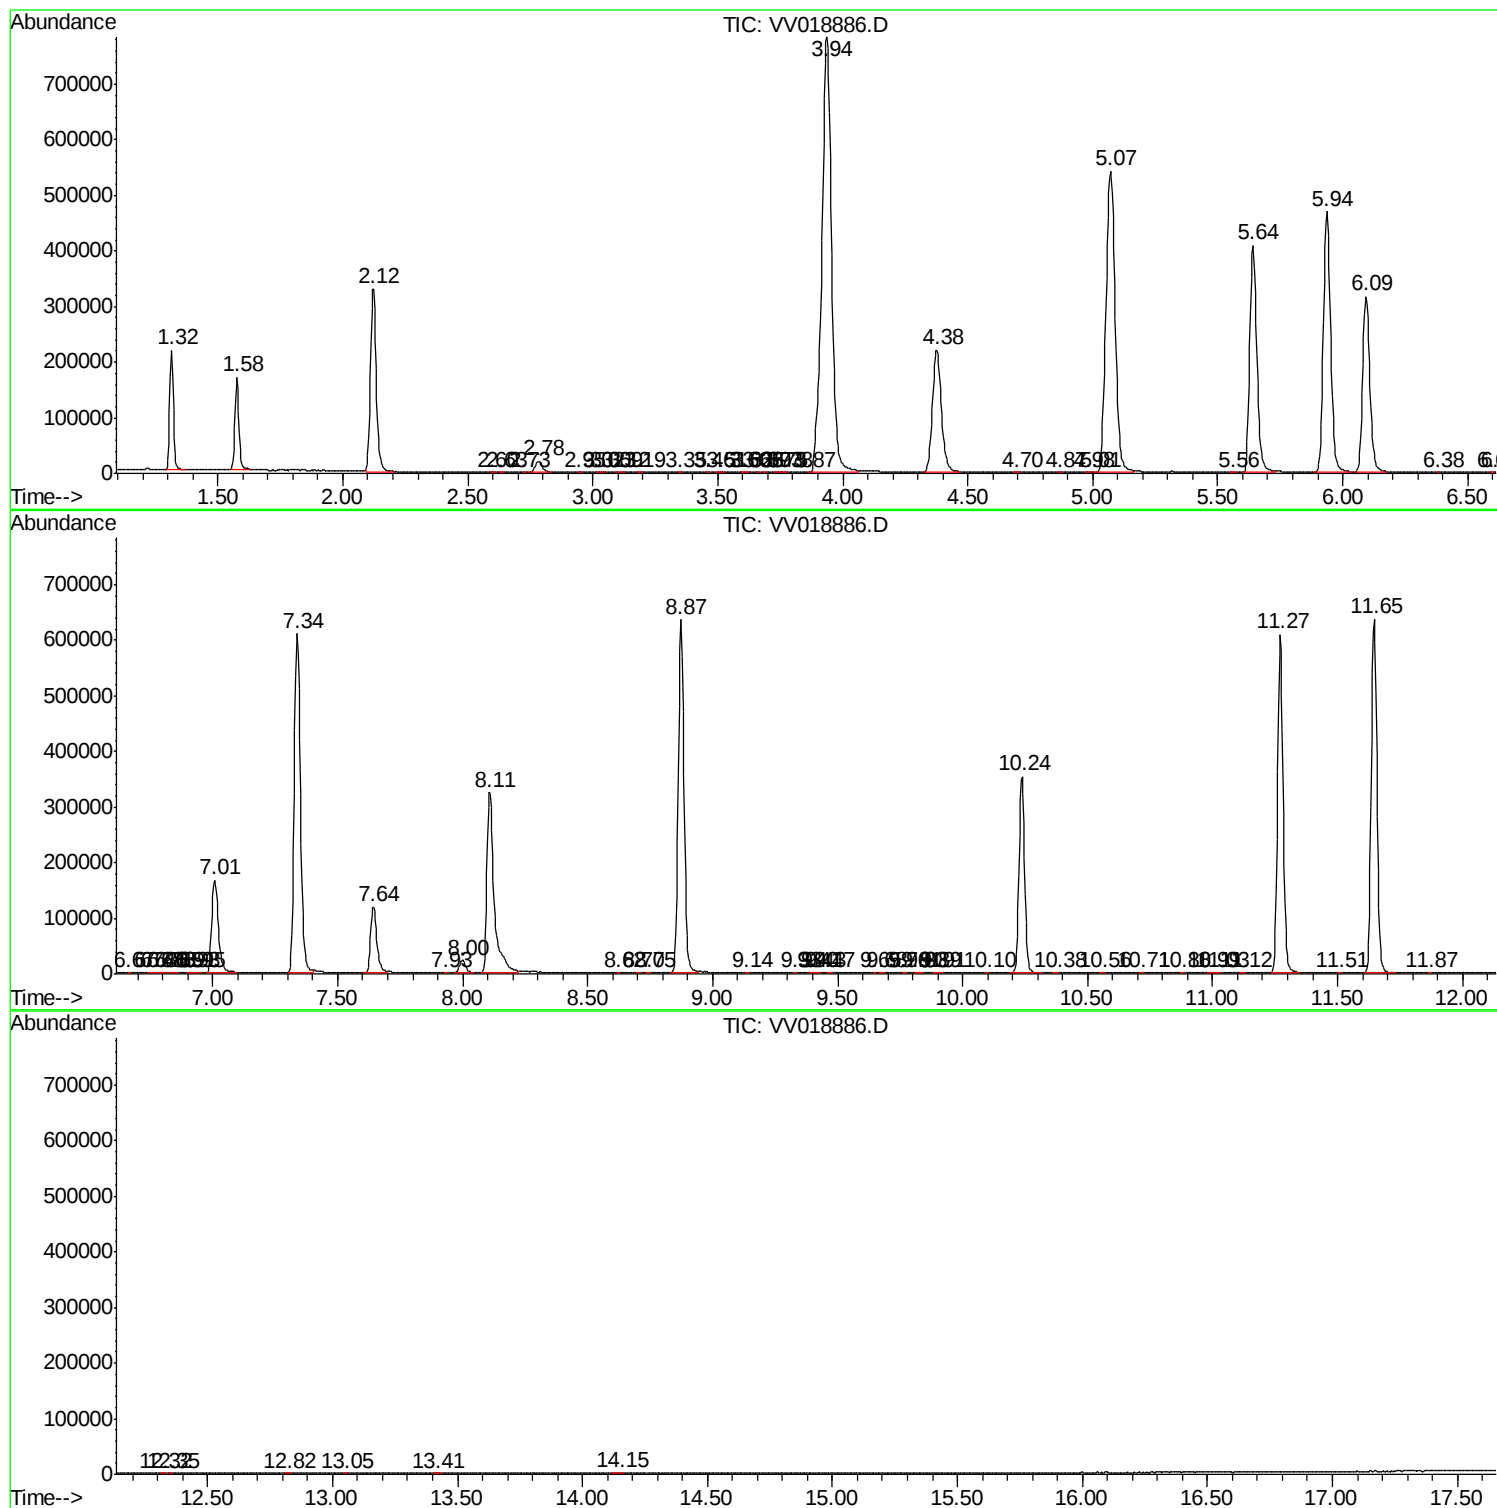

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV101320\
Data File : VV018886.D
Acq On : 13 Oct 2020 19:00
Operator : SY/MD
Sample : L4351-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV101320\
Data File : VV018886.D
Acq On : 13 Oct 2020 19:00
Operator : SY/MD
Sample : L4351-05
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AJ2

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM100820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc