


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV101320\
 Data File : VV018868.D
 Acq On : 13 Oct 2020 09:03
 Operator : SY/MD
 Sample : BFB73
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB73

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM100820WMA.M
 Title : VOC Analysis
 Last Update : Wed Oct 14 10:35:42 2020

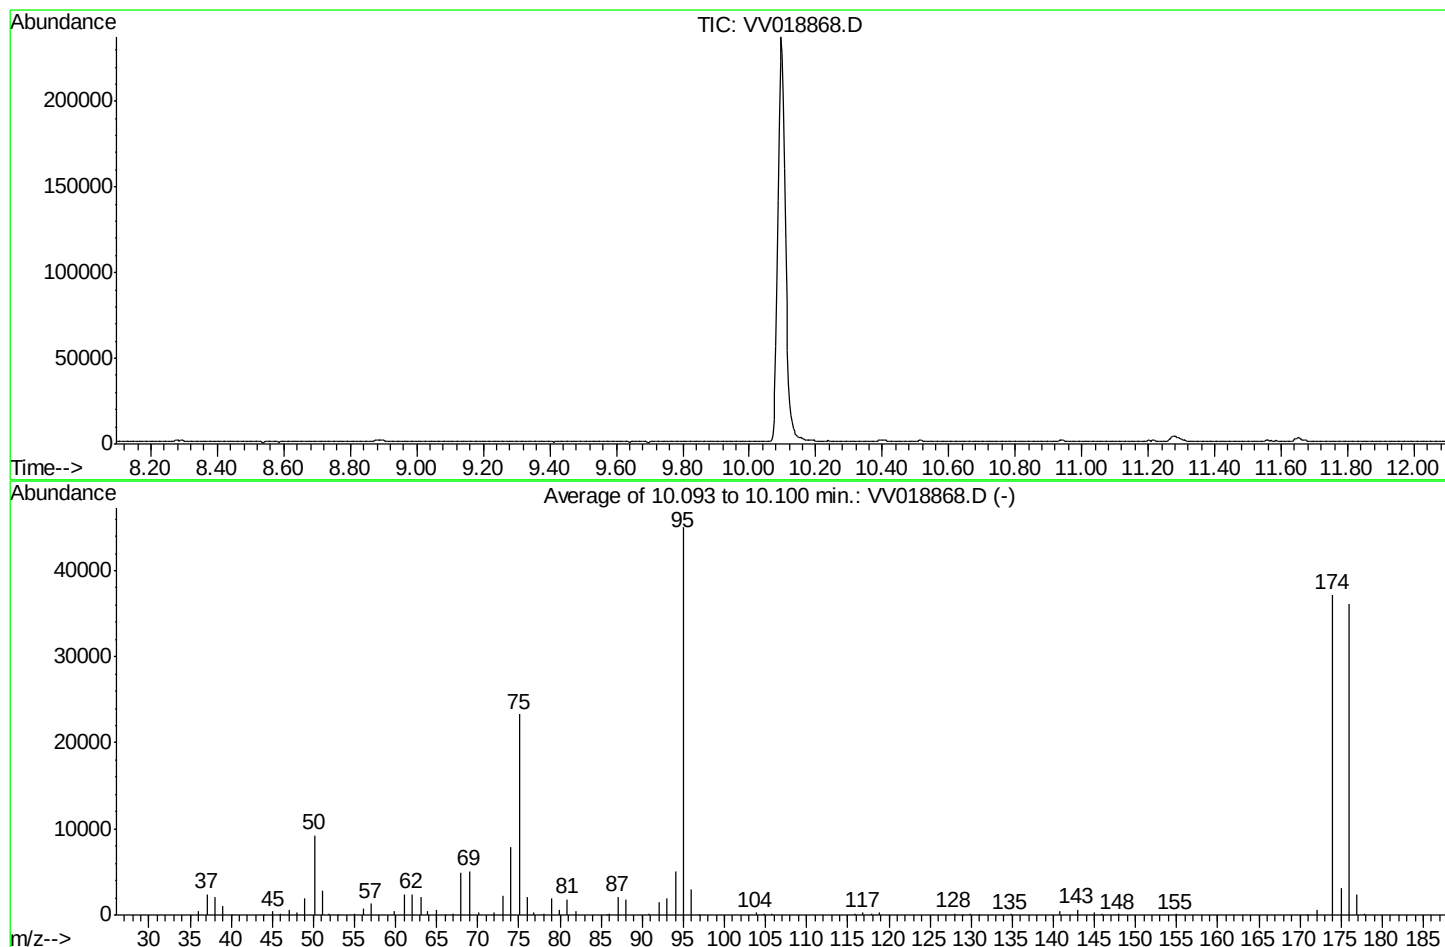

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	9273	PASS
75	95	30	80	51.7	23272	PASS
95	95	100	100	100.0	45024	PASS
96	95	5	9	6.8	3050	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.6	37192	PASS
175	174	5	9	8.4	3108	PASS
176	174	95	101	97.3	36194	PASS
177	176	5	9	6.7	2433	PASS

m/z	Abundance
36.10	468.0
37.10	2334.0
38.00	2033.0
39.00	988.0
40.00	365.0
44.00	1279.0
45.10	355.0
46.00	145.0
47.00	635.0
48.00	339.0
49.00	1995.0
50.10	9149.0
51.00	2805.0
51.90	145.0
52.90	111.0
54.90	170.0
56.00	788.0
57.00	1249.0
59.90	454.0
61.00	2368.0
62.00	2419.0
63.10	2120.0
64.00	490.0
65.00	532.0
66.00	111.0
66.90	177.0
68.00	4789.0
69.00	5211.0
70.00	366.0
71.90	263.0
73.00	2200.0
74.00	7600.0
75.00	22936.0
76.00	2044.0
76.90	331.0
78.00	201.0
78.90	1800.0
79.90	552.0
80.90	1762.0
81.90	484.0
85.70	111.0
87.00	1938.0
87.90	1871.0
90.90	224.0
92.00	1425.0
93.00	1875.0
94.00	4948.0
95.00	44144.0
96.00	3016.0
103.90	209.0
104.80	126.0
105.80	157.0
115.90	203.0
116.90	296.0
117.90	152.0
118.90	294.0
127.90	181.0
129.90	198.0
131.00	103.0
134.80	128.0
140.80	431.0
142.90	666.0
144.90	209.0
145.90	132.0
147.90	124.0
154.90	155.0
172.00	596.0
174.00	35240.0
175.00	3044.0
176.00	34216.0
176.90	2379.0
177.80	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
36.10	478.0
37.10	2532.0
38.00	2142.0
39.00	1067.0
40.00	329.0
44.00	1258.0
45.10	394.0
46.00	119.0
47.00	663.0
48.00	311.0
49.00	2060.0
50.10	9605.0
51.00	2903.0
51.90	155.0
55.00	173.0
56.10	838.0
57.00	1362.0
59.90	465.0
61.00	2535.0
62.00	2512.0
63.10	2189.0
63.90	503.0
65.00	558.0
67.00	145.0
68.00	5053.0
69.00	5221.0
70.10	378.0
72.00	304.0
73.00	2283.0
74.00	8081.0
75.00	24120.0
76.00	2194.0
76.90	342.0
78.00	174.0
78.90	1937.0
79.90	543.0
80.90	1917.0
81.90	437.0
86.00	126.0
87.00	2220.0
88.00	1890.0
90.80	186.0
92.00	1491.0
93.00	2004.0
94.00	5178.0
95.00	46504.0
96.00	3214.0
103.80	236.0
104.80	121.0
105.80	198.0
115.90	204.0
116.90	294.0
117.90	150.0
118.90	290.0
128.00	198.0
128.90	108.0
129.80	203.0
134.90	135.0
140.80	460.0
142.90	663.0
145.00	250.0
146.00	133.0
147.90	144.0
154.90	106.0
170.80	102.0
172.00	677.0
174.00	38392.0
175.00	3206.0
176.00	37512.0
176.90	2509.0
177.80	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
36.00	429.0
37.00	2463.0
38.00	2164.0
39.00	1003.0
40.00	334.0
44.00	1189.0
45.10	404.0
46.00	107.0
47.00	636.0
47.90	284.0
49.00	1953.0
50.10	9066.0
51.10	2818.0
51.90	160.0
55.00	155.0
56.10	784.0
57.00	1337.0
59.90	426.0
61.00	2349.0
62.00	2328.0
63.00	2078.0
63.90	457.0
65.00	489.0
66.90	123.0
68.00	4898.0
69.00	4747.0
70.00	353.0
72.00	280.0
73.00	2127.0
74.00	7770.0
75.10	22760.0
76.00	2065.0
76.80	340.0
78.90	1857.0
79.90	511.0
80.90	1873.0
81.90	422.0
86.00	153.0
87.00	2129.0
88.00	1670.0
90.80	158.0
92.00	1359.0
93.00	1877.0
94.00	5081.0
95.00	44424.0
96.00	2922.0
96.90	106.0
103.80	253.0
104.80	109.0
105.80	219.0
115.90	199.0
116.80	303.0
117.80	174.0
118.90	297.0
128.00	198.0
129.80	164.0
134.90	175.0
140.90	444.0
142.90	614.0
145.00	256.0
147.90	142.0
170.90	105.0
172.00	692.0
174.00	37944.0
175.00	3074.0
176.00	36856.0
176.90	2412.0
177.80	138.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

Scan 2789 (10.058 min): VV018868.D
BFB73

m/z	Abundance
40.00	332.0
44.00	1192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73