

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101321\
 Data File : VV022762.D
 Acq On : 13 Oct 2021 15:22
 Operator : SY/MD
 Sample : M4022-25
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022762.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	77	82	97	rVB	61490	69718	16.67%	2.083%
2	1.564	157	163	177	rBV	57900	66860	15.99%	1.998%
3	2.105	320	331	348	rBV	108674	160337	38.34%	4.790%
4	2.507	447	456	469	rBV	7639	13314	3.18%	0.398%
5	3.928	883	898	913	rBV2	22615	88079	21.06%	2.632%
6	4.349	1010	1029	1055	rBV	76854	193582	46.28%	5.784%
7	5.050	1231	1247	1273	rBV2	169964	418243	100.00%	12.496%
8	5.619	1412	1424	1447	rBV	128585	267380	63.93%	7.989%
9	6.072	1550	1565	1590	rBV	96614	204608	48.92%	6.113%
10	6.989	1839	1850	1871	rBV2	38162	75070	17.95%	2.243%
11	7.317	1941	1952	1970	rBV	186399	329715	78.83%	9.851%
12	7.625	2037	2048	2070	rBV2	22554	43547	10.41%	1.301%
13	8.095	2179	2194	2216	rBV	175827	343046	82.02%	10.249%
14	8.854	2419	2430	2455	rBV	207100	336671	80.50%	10.059%
15	10.217	2843	2854	2874	rBV	70386	111488	26.66%	3.331%
16	11.249	3164	3175	3192	rBV	196570	305371	73.01%	9.124%
17	11.625	3281	3292	3312	rBV	189222	293424	70.16%	8.767%
18	15.384	4454	4461	4469	rBV6	5939	7719	1.85%	0.231%
19	17.101	4985	4995	5007	rBV	11252	18883	4.51%	0.564%




Sum of corrected areas: 3347055

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101321\
Data File : VV022762.D
Acq On : 13 Oct 2021 15:22
Operator : SY/MD
Sample : M4022-25
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

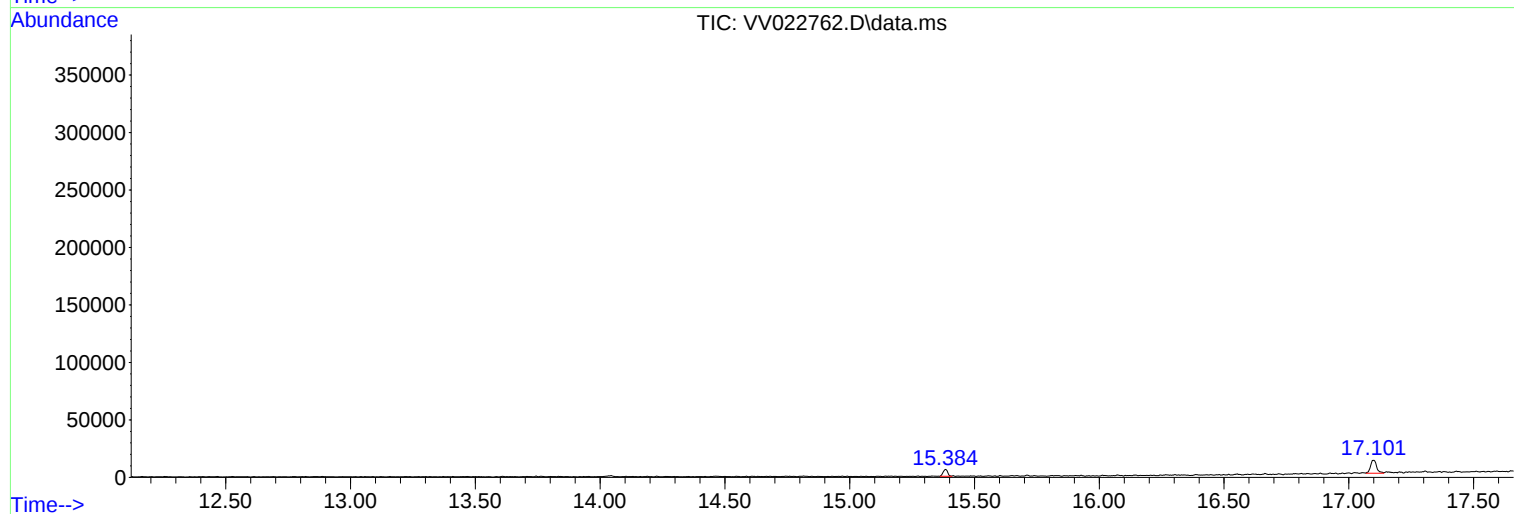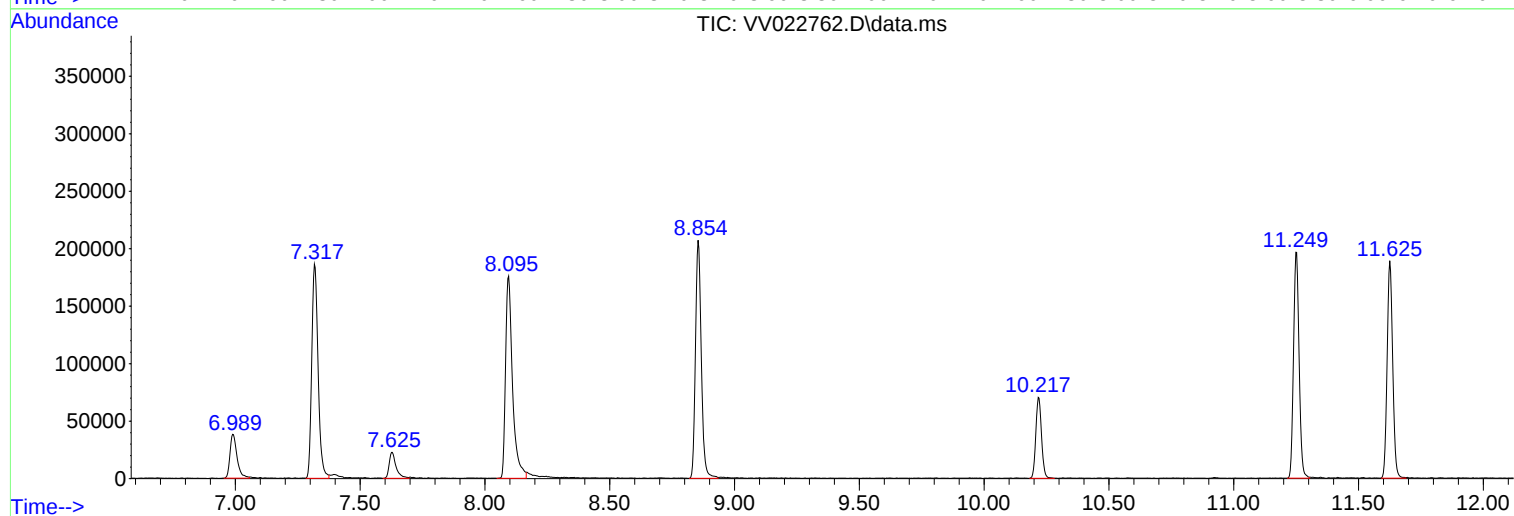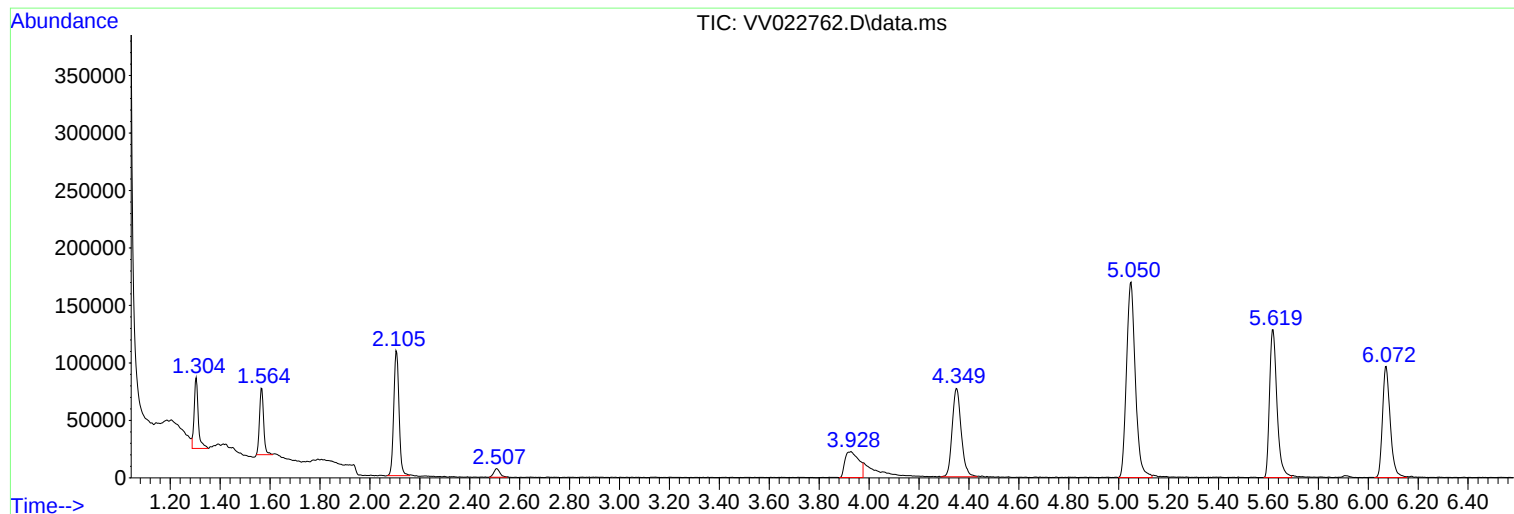

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101321\
Data File : VV022762.D
Acq On : 13 Oct 2021 15:22
Operator : SY/MD
Sample : M4022-25
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101321\
Data File : VV022762.D
Acq On : 13 Oct 2021 15:22
Operator : SY/MD
Sample : M4022-25
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
