

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101321\
 Data File : VV022763.D
 Acq On : 13 Oct 2021 15:50
 Operator : SY/MD
 Sample : M4098-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022763.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	58879	61952	14.73%	1.813%
2	1.565	157	163	172	rBV	56907	63784	15.16%	1.867%
3	2.105	320	331	347	rBV	109354	157860	37.53%	4.620%
4	2.507	446	456	467	rBV2	11188	18411	4.38%	0.539%
5	3.928	884	898	934	rBV2	22764	120796	28.72%	3.535%
6	4.349	1013	1029	1053	rBV	75493	190684	45.33%	5.581%
7	5.047	1229	1246	1277	rBV2	164965	420616	100.00%	12.310%
8	5.616	1411	1423	1457	rBV	132082	273564	65.04%	8.006%
9	6.069	1552	1564	1586	rBV	97963	203911	48.48%	5.968%
10	6.989	1839	1850	1873	rBV2	40078	78587	18.68%	2.300%
11	7.317	1940	1952	1971	rBV	189629	331024	78.70%	9.688%
12	7.625	2039	2048	2069	rBV2	23321	44613	10.61%	1.306%
13	8.092	2183	2193	2226	rBV	182228	359609	85.50%	10.525%
14	8.854	2419	2430	2449	rBV	213132	345273	82.09%	10.105%
15	10.217	2843	2854	2874	rBV	71147	113966	27.10%	3.335%
16	11.249	3165	3175	3193	rBV	205116	316935	75.35%	9.276%
17	11.625	3278	3292	3312	rBV	192198	300265	71.39%	8.788%
18	15.384	4453	4461	4470	rBV5	4814	6366	1.51%	0.186%
19	17.098	4985	4994	5004	rBV3	5783	8632	2.05%	0.253%




Sum of corrected areas: 3416848

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101321\
Data File : VV022763.D
Acq On : 13 Oct 2021 15:50
Operator : SY/MD
Sample : M4098-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

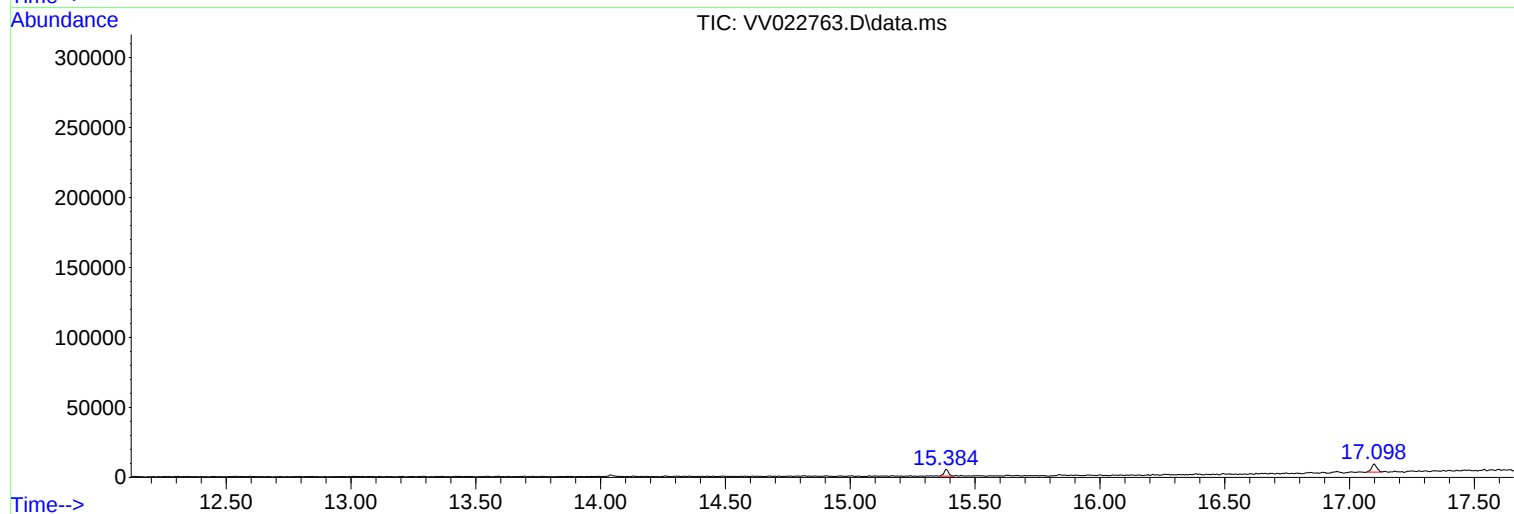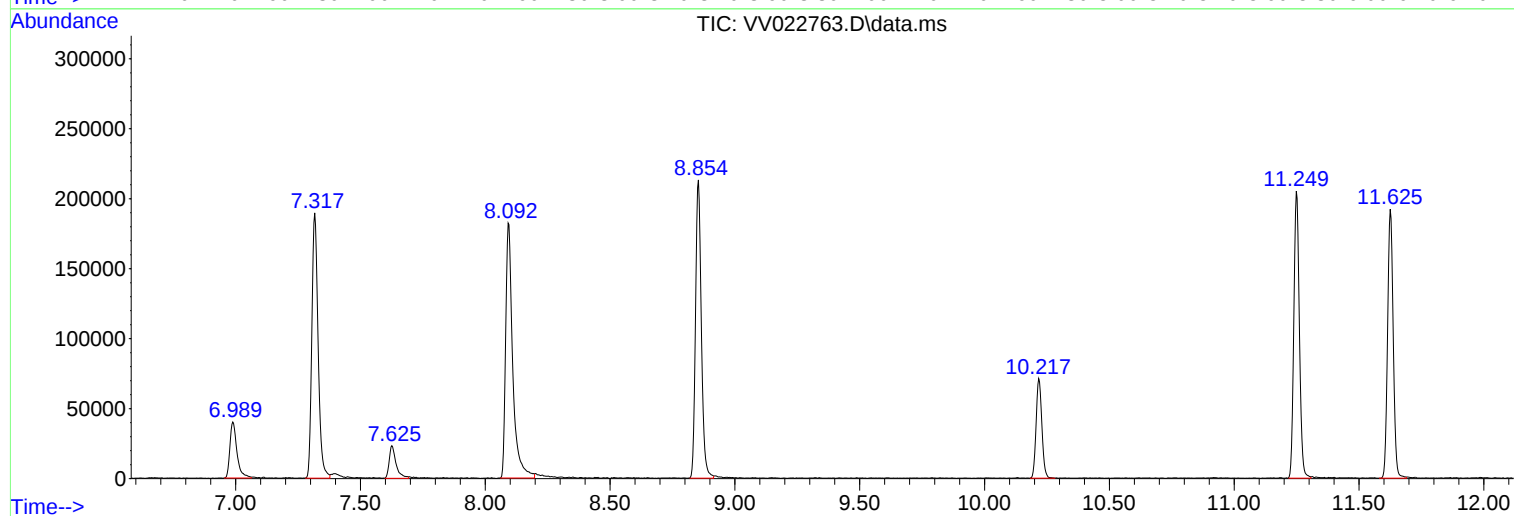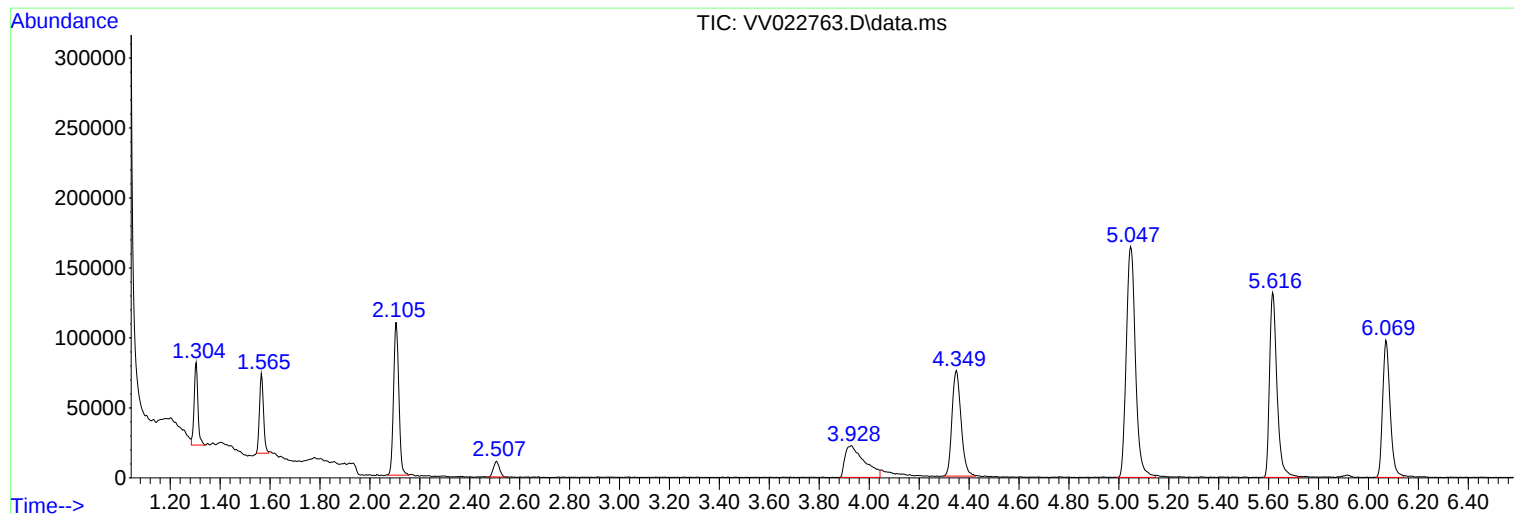

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101321\
Data File : VV022763.D
Acq On : 13 Oct 2021 15:50
Operator : SY/MD
Sample : M4098-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101321\
Data File : VV022763.D
Acq On : 13 Oct 2021 15:50
Operator : SY/MD
Sample : M4098-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
