
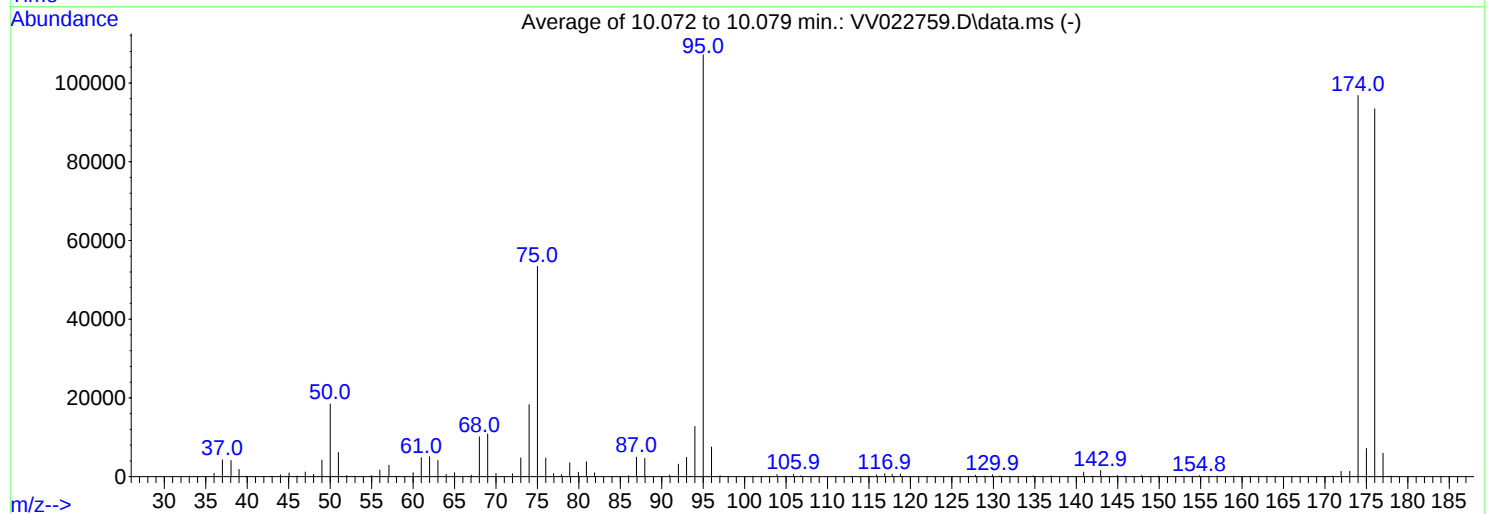


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101321\
 Data File : VV022759.D
 Acq On : 13 Oct 2021 10:19
 Operator : SY/MD
 Sample : BFB214
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB214

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR100721WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Oct 15 06:41:28 2021

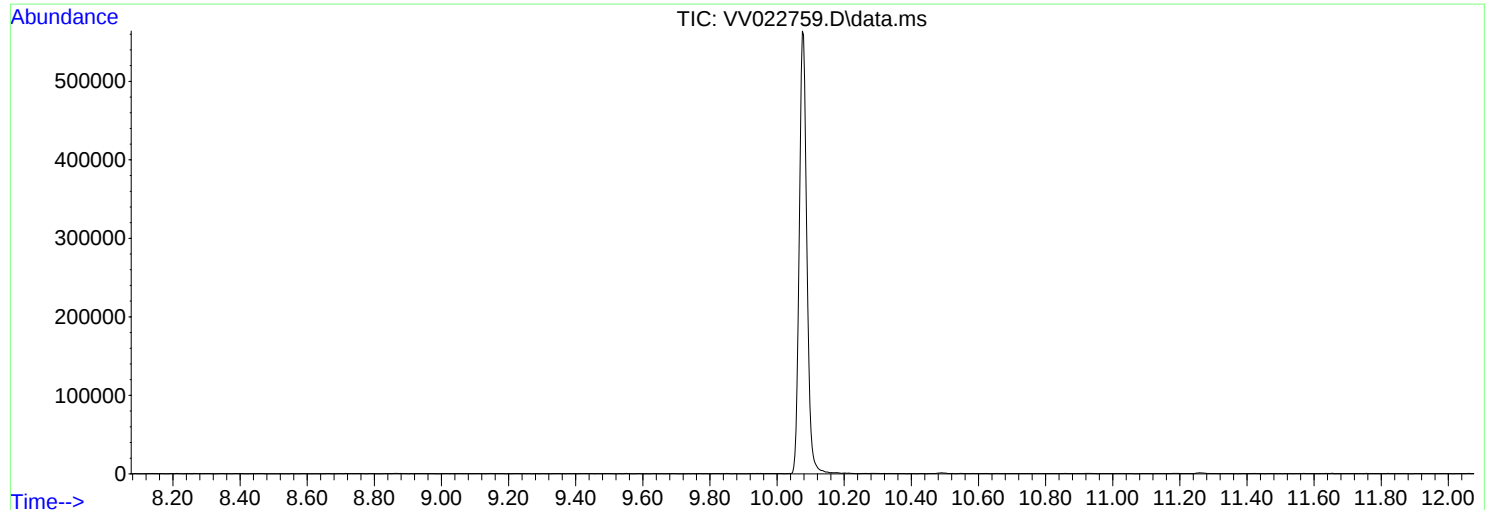

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	18437	PASS
75	95	30	80	49.8	53395	PASS
95	95	100	100	100.0	107144	PASS
96	95	5	9	7.0	7540	PASS
173	174	0.00	2	1.4	1342	PASS
174	95	50	120	90.4	96832	PASS
175	174	5	9	7.4	7155	PASS
176	174	95	105	96.5	93453	PASS
177	176	5	10	6.4	5941	PASS

m/z	Abundance
36.00	869.0
37.00	4386.0
38.00	4304.0
39.00	1908.0
40.00	209.0
41.90	101.0
42.80	112.0
44.00	699.0
45.10	971.0
46.00	158.0
47.00	1239.0
48.00	592.0
49.00	4384.0
50.00	19128.0
51.00	6423.0
52.00	300.0
52.90	134.0
55.00	313.0
56.00	1744.0
57.10	3023.0
57.90	155.0
60.00	1089.0
61.00	4952.0
62.00	5253.0
63.00	4267.0
64.00	603.0
65.00	1110.0
66.00	124.0
67.10	312.0
68.00	10483.0
69.00	11262.0
70.00	828.0
72.00	781.0
73.00	4971.0
74.00	19064.0
75.00	55440.0
76.00	4896.0
76.90	835.0
77.90	579.0
78.90	3654.0
80.00	1193.0
80.90	3856.0
81.90	1009.0
82.90	113.0
86.00	267.0
86.90	5201.0
87.90	4696.0
91.00	442.0
92.00	3266.0
93.00	5029.0
94.00	13162.0
95.00	111160.0
96.00	7809.0
97.00	244.0
103.90	562.0
104.90	164.0
105.90	625.0
106.80	260.0
110.00	107.0
111.00	144.0
112.80	123.0
115.00	158.0
115.90	457.0
116.90	758.0
117.80	636.0
118.80	672.0
127.90	391.0
128.90	166.0
129.90	509.0
130.80	230.0
134.80	217.0
137.00	220.0
140.90	1197.0
141.90	152.0
142.90	1592.0
143.80	130.0
144.90	356.0
145.90	187.0
146.80	104.0
147.90	331.0
148.80	108.0
149.90	162.0
152.80	104.0
154.90	286.0
157.00	179.0
158.90	195.0
161.00	132.0
171.00	140.0
172.00	1391.0
173.00	1364.0
174.00	100224.0
175.00	7440.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

176.00	96464.0
177.00	6195.0
177.90	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

m/z	Abundance
36.00	818.0
37.00	4410.0
38.00	4260.0
39.00	1836.0
40.00	220.0
41.90	112.0
44.00	754.0
45.10	922.0
46.10	219.0
47.00	1203.0
48.00	582.0
49.00	4269.0
50.00	18744.0
51.00	6270.0
52.00	293.0
52.90	187.0
55.00	335.0
56.00	1665.0
57.10	2905.0
57.90	179.0
60.00	1009.0
61.00	4943.0
62.00	5169.0
63.00	3978.0
64.00	565.0
65.00	972.0
66.00	102.0
67.00	295.0
68.00	10240.0
69.00	10999.0
70.00	807.0
72.00	722.0
73.00	4864.0
74.00	18336.0
75.00	54184.0
76.00	4668.0
76.90	793.0
77.90	573.0
78.90	3491.0
79.90	1265.0
80.90	3824.0
81.90	1031.0
86.00	261.0
87.00	5190.0
88.00	4862.0
90.90	396.0
92.00	3315.0
93.00	5121.0
94.00	13076.0
95.00	108264.0
96.00	7777.0
97.10	226.0
103.90	540.0
104.80	155.0
105.90	575.0
106.80	230.0
109.60	122.0
111.00	131.0
112.00	110.0
112.80	149.0
115.00	147.0
115.90	456.0
116.90	773.0
117.80	596.0
118.80	623.0
127.90	376.0
128.90	171.0
129.90	489.0
130.80	210.0
134.80	224.0
136.90	242.0
140.90	1164.0
142.10	146.0
143.00	1496.0
143.80	134.0
145.00	332.0
145.90	172.0
147.90	330.0
149.90	169.0
154.80	282.0
157.00	166.0
158.90	164.0
160.90	143.0
170.90	159.0
172.00	1490.0
173.00	1403.0
174.00	101488.0
175.00	7421.0
176.00	98192.0
177.00	6095.0
178.00	183.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

m/z	Abundance
39.90	101.0
44.00	237.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214

m/z	Abundance
36.00	833.0
37.00	4009.0
38.10	3809.0
39.00	1725.0
39.90	204.0
42.80	106.0
44.00	634.0
45.00	896.0
46.00	142.0
47.00	1126.0
48.00	570.0
49.00	3990.0
50.00	17440.0
51.00	5709.0
52.00	265.0
54.90	254.0
56.00	1601.0
57.10	2746.0
58.20	151.0
60.00	968.0
61.00	4568.0
62.00	4846.0
63.00	4029.0
64.00	540.0
65.00	1036.0
65.90	111.0
67.10	361.0
68.00	9602.0
69.00	10362.0
70.00	764.0
72.00	709.0
73.00	4405.0
74.00	17528.0
75.00	50560.0
76.00	4534.0
77.00	758.0
77.90	494.0
78.90	3498.0
80.00	1007.0
80.90	3665.0
81.90	912.0
82.90	121.0
86.00	239.0
86.90	4536.0
88.00	4296.0
90.90	436.0
92.00	2889.0
93.00	4459.0
94.00	12005.0
95.00	102008.0
96.00	7034.0
97.00	239.0
103.90	544.0
105.00	156.0
105.90	572.0
106.80	233.0
111.00	130.0
112.90	109.0
114.90	146.0
115.90	403.0
116.90	714.0
117.80	539.0
118.80	645.0
127.80	358.0
128.90	163.0
129.90	483.0
130.80	218.0
131.00	223.0
134.80	185.0
137.00	196.0
140.90	1077.0
141.80	163.0
142.90	1497.0
144.90	354.0
145.80	200.0
147.90	289.0
149.90	153.0
152.80	110.0
154.90	238.0
157.00	198.0
159.00	186.0
161.00	108.0
171.00	162.0
171.90	1203.0
173.00	1258.0
174.00	88784.0
175.00	6603.0
176.00	85704.0
177.00	5534.0
177.90	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB214